Data File C:\Chem32\2\Data\Gamma\20251005_Calibration_N2O-Standards-100ppm-1.D
Sample Name: Calibration_N2O-Standards-600ppm-1

===

Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : Green House Gas GC   Location :   1 (F)
Injection Date : 10/5/2025 12:44:19 PM
                                              Inj Volume : Manually
Method   : C:\Chem32\2\Methods\Gamma-N2O-2.M
Last changed   : 10/5/2025 11:52:09 AM by SYSTEM
                  (modified after loading)

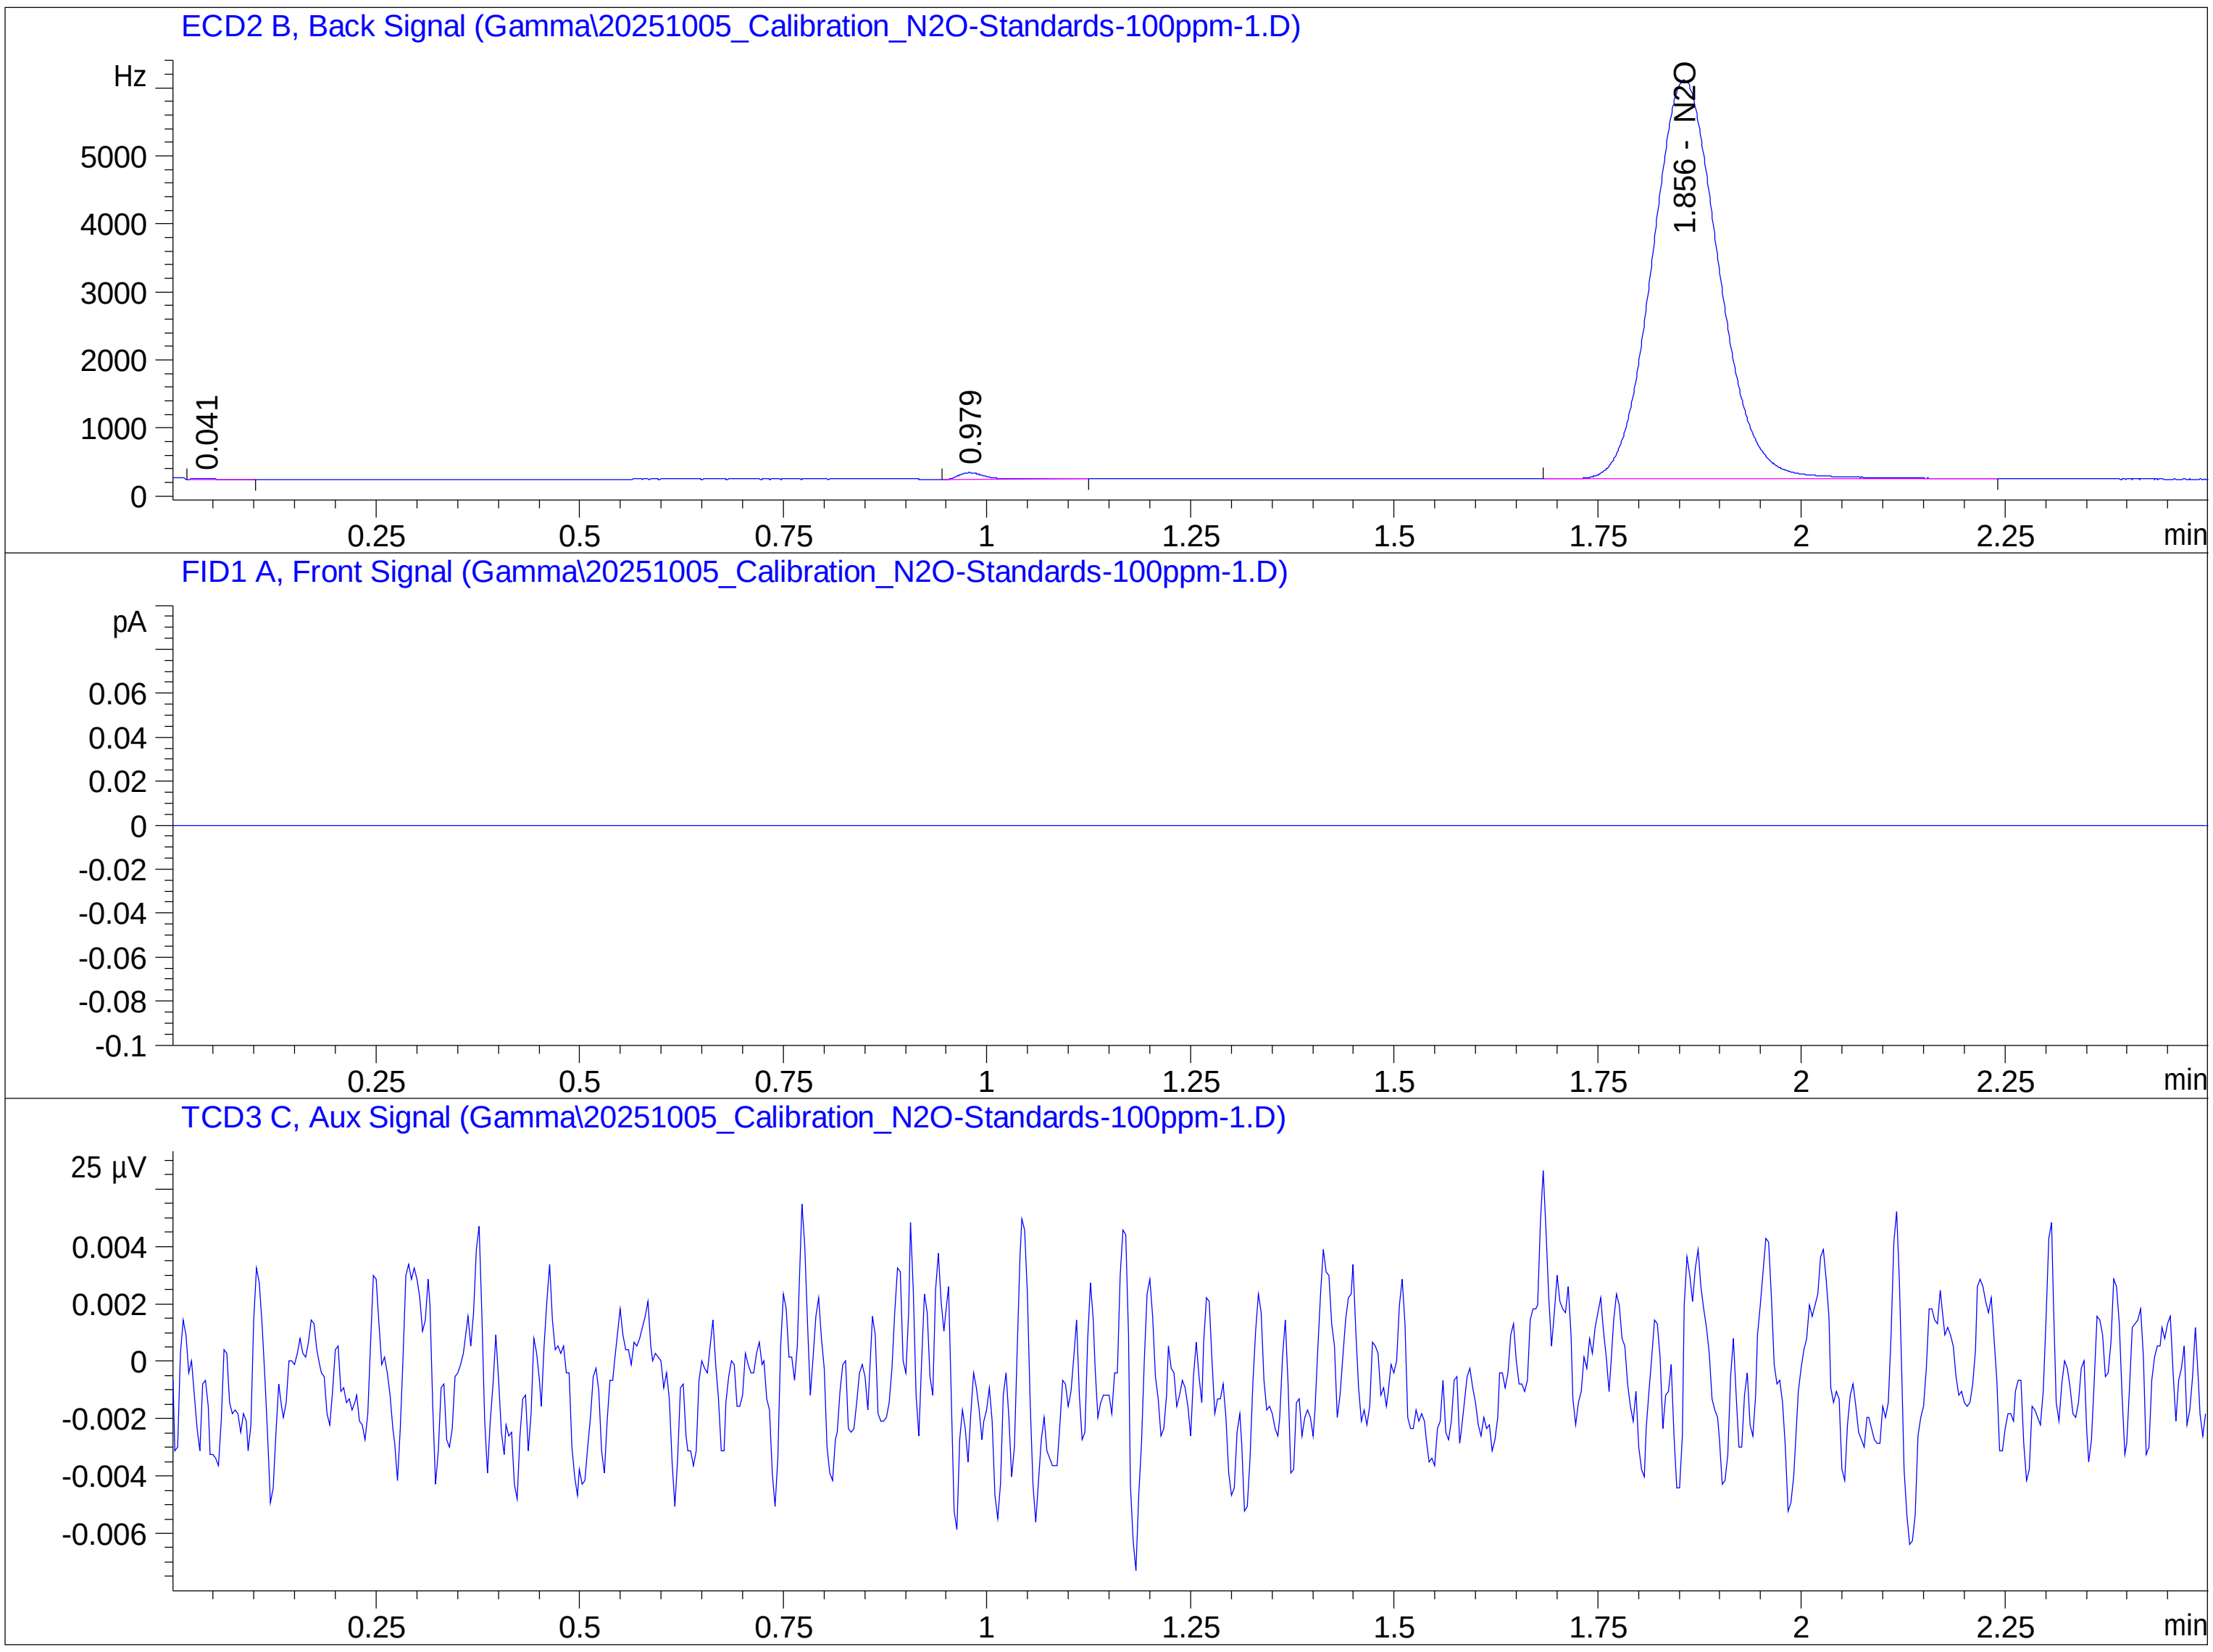

===

External Standard Report

===

Sorted By   :   Signal
Calib. Data Modified :   10/5/2025 11:52:09 AM
Multiplier   :   1.0000
Dilution   :   1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: ECD2 B, Back Signal

RetTime [min]	Type	Area [Hz*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.856	BBA	3.33621e4	3.23624e-3	107.96762		N2O
2.847		-	-	-		NO2

Totals : 107.96762

Signal 2: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.141		-	-	-		Methane
1.945		-	-	-		CO2

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

RetTime [min]	Type	Area [25 µV*s]	Amt/Area	Amount [ng/ul]	Grp	Name
3.272		-	-	-		CO2
4.177		-	-	-		NO2
5.338		-	-	-		Oxygen
6.396		-	-	-		Nitrogen
8.853		-	-	-		Methane

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

===

*** End of Report ***