

Sample Name: SAMPLE_20251001-1215PM-ELECDON-GOWN311A


=====

Acq. Operator : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : Green House Gas GC Location : 1 (F)
Injection Date : 10/1/2025 5:53:25 PM
Inj Volume : Manually

Acq. Method : C:\Chem32\2\Methods\Gamma-N20-2.M
Last changed : 10/1/2025 4:48:35 PM by SYSTEM
(modified after loading)

Analysis Method : C:\Chem32\2\Methods\Gamma-N20-2.M
Last changed : 10/1/2025 5:56:17 PM by SYSTEM
(modified after loading)

Additional Info : Peak(s) manually integrated

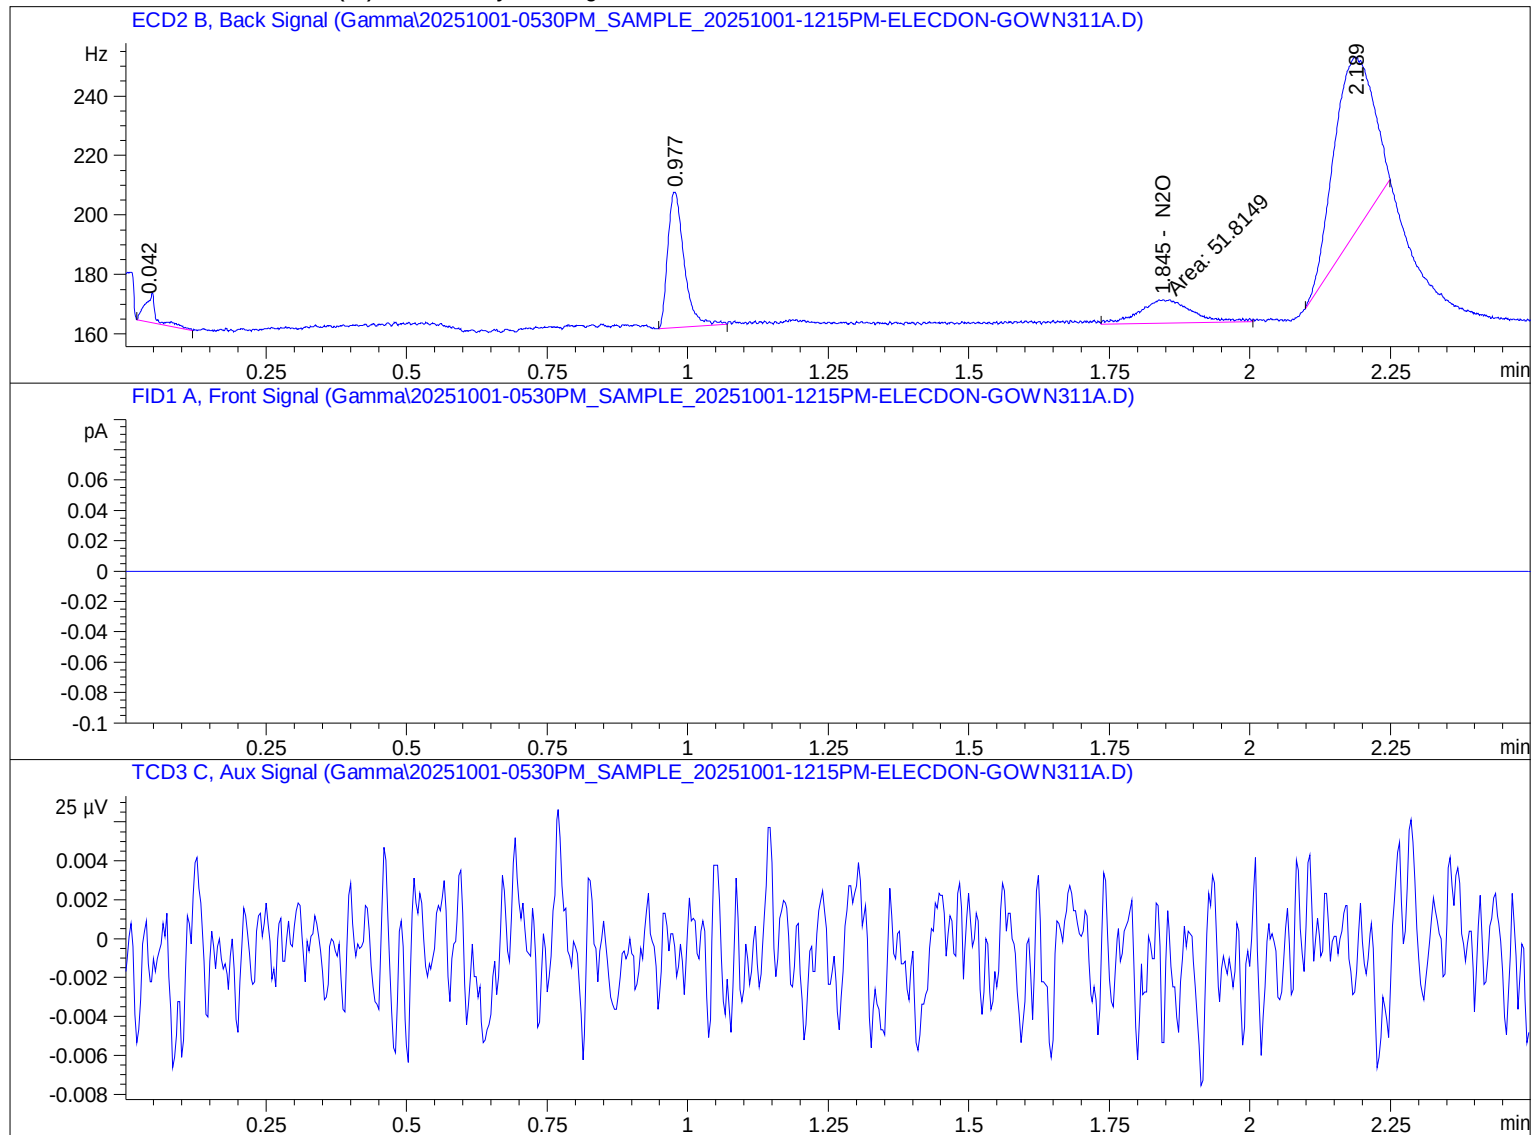

=====

External Standard Report

=====

Sorted By : Signal
Calib. Data Modified : 10/1/2025 2:07:40 PM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Sample Name: SAMPLE_20251001-1215PM-ELECDON-GOWN311A

Signal 1: ECD2 B, Back Signal

RetTime [min]	Type	Area [Hz*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.845	MM	51.81486	3.11253e-3	1.61275e-1		N2O
2.847		-	-	-		N2O2

Totals : 1.61275e-1

Signal 2: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.141		-	-	-		Methane
1.945		-	-	-		CO2

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

RetTime [min]	Type	Area [25 μ V*s]	Amt/Area	Amount [ng/ul]	Grp	Name
3.272		-	-	-		CO2
4.177		-	-	-		N2O2
5.338		-	-	-		Oxygen
6.396		-	-	-		Nitrogen
8.853		-	-	-		Methane

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

*** End of Report ***