


Sample Name: SAMPLE_20250921-1245PM-D87LIQ-CL1

=====
Acq. Operator : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : Green House Gas GC Location : 1 (F)
Injection Date : 9/25/2025 9:18:35 PM
Inj Volume : Manually
Acq. Method : C:\Chem32\2\Methods\Gammaamma-N20-2.M
Last changed : 9/25/2025 6:08:39 PM by SYSTEM
(modified after loading)
Analysis Method : C:\Chem32\2\Methods\Gammaamma-N20-2.M
Last changed : 9/25/2025 9:21:19 PM by SYSTEM
(modified after loading)
Additional Info : Peak(s) manually integrated

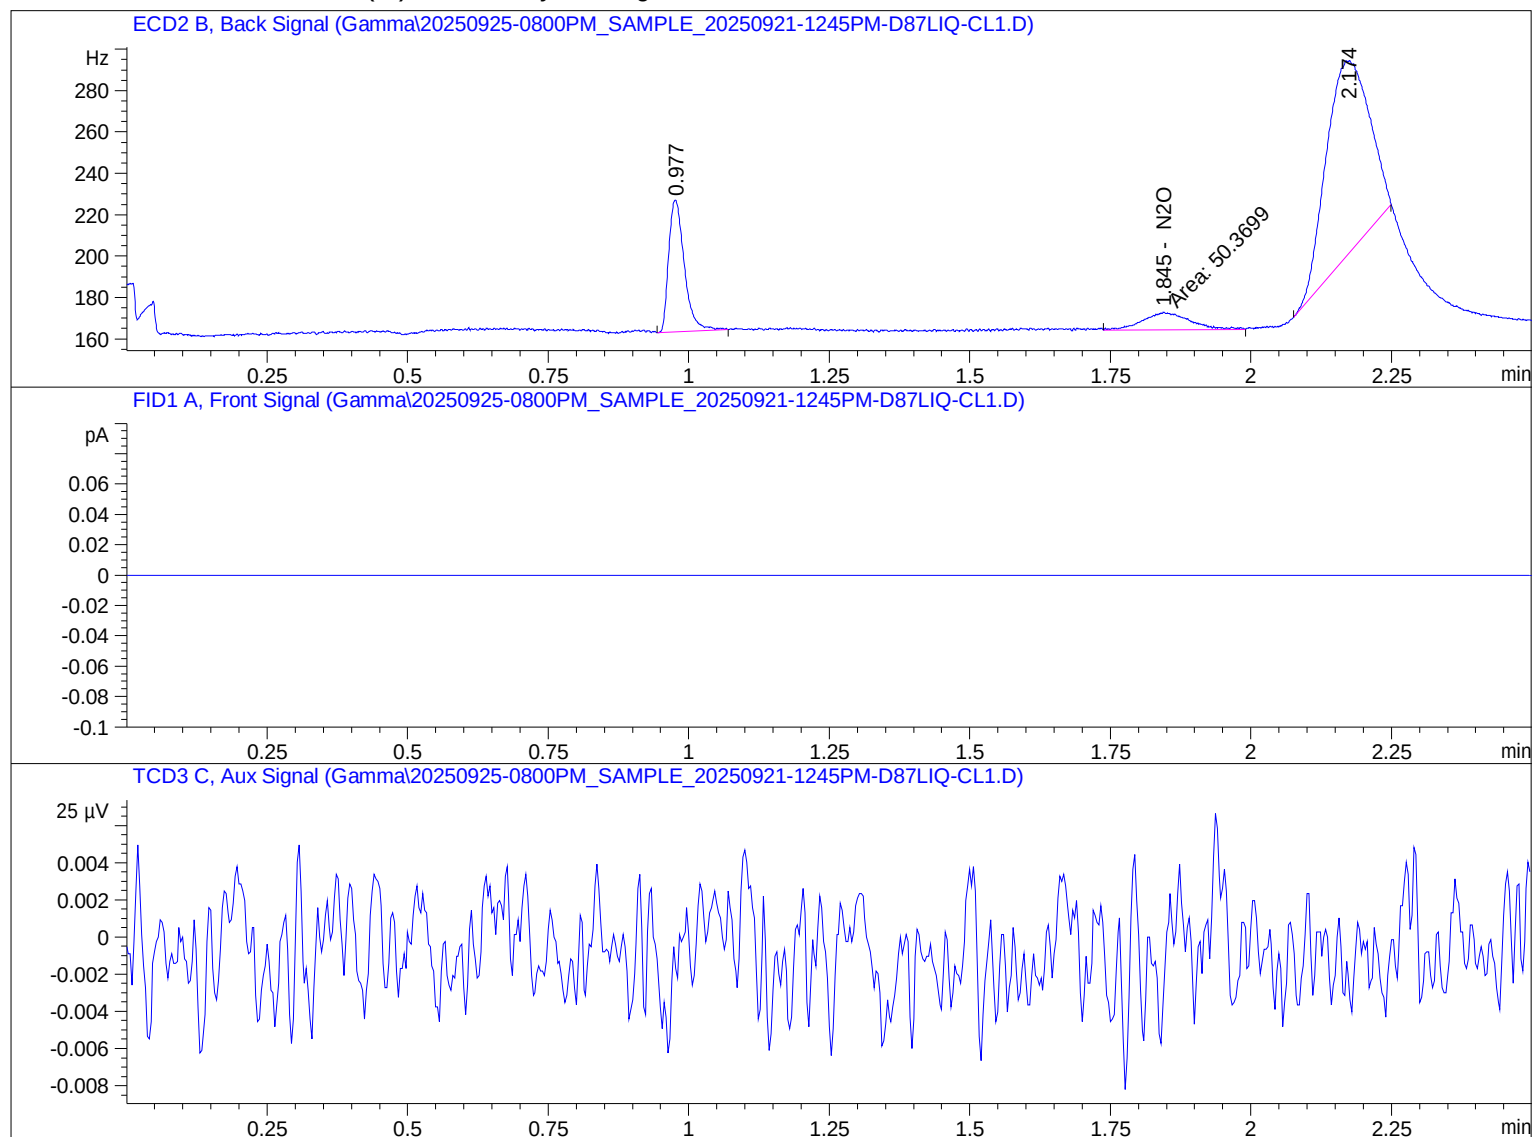

=====
External Standard Report
=====

Sorted By : Signal
Calib. Data Modified : 9/25/2025 2:17:23 PM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: ECD2 B, Back Signal

RetTime [min]	Type	Area [Hz*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.845	MM	50.36994	3.75039e-3	1.88907e-1		N2O
2.847		-	-	-		N02

Totals : 1.88907e-1

Signal 2: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.141		-	-	-		Methane
1.945		-	-	-		C02

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

RetTime [min]	Type	Area [25 µV*s]	Amt/Area	Amount [ng/ul]	Grp	Name
3.272		-	-	-		C02
4.177		-	-	-		N02
5.338		-	-	-		Oxygen
6.396		-	-	-		Nitrogen
8.853		-	-	-		Methane

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====
*** End of Report ***