


Sample Name: SAMPLE_20251001-1215PM-ELECDON-GOWN311A

```
=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : Green House Gas GC           Location :    1  (F)
Injection Date  : 10/1/2025 2:37:11 PM
                                           Inj Volume : Manually

Acq. Method     : C:\Chem32\2\Methods\Gammaamma-N20-2.M
Last changed    : 10/1/2025 2:33:52 PM by SYSTEM
                  (modified after loading)
Analysis Method : C:\Chem32\2\Methods\Gammaamma-N20-2.M
Last changed    : 10/1/2025 2:39:58 PM by SYSTEM
                  (modified after loading)
Additional Info  : Peak(s) manually integrated
=====
```

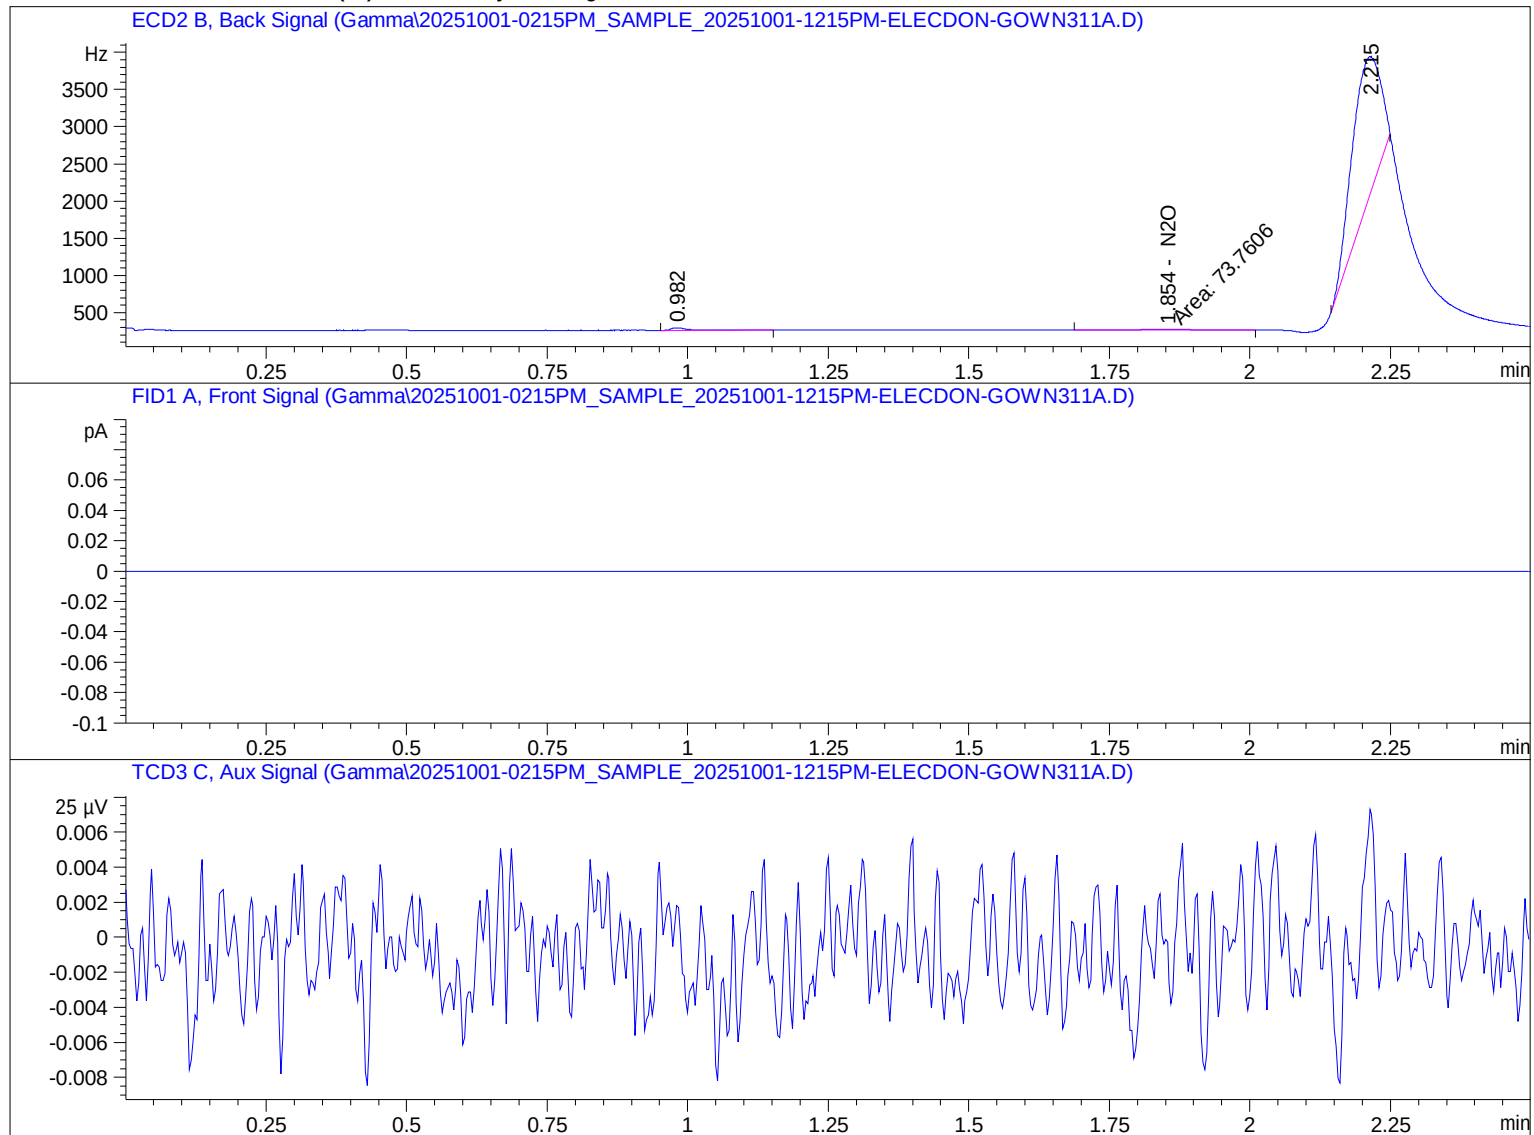

```
=====
External Standard Report
=====
```

```
Sorted By      :      Signal
Calib. Data Modified :    10/1/2025 2:07:40 PM
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Sample Name: SAMPLE_20251001-1215PM-ELECDON-GOWN311A

Signal 1: ECD2 B, Back Signal

RetTime [min]	Type	Area [Hz*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.854	MM	73.76058	3.11253e-3	2.29582e-1	N20	
2.847		-	-	-	N02	

Totals : 2.29582e-1

Signal 2: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.141		-	-	-		Methane
1.945		-	-	-		CO2

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

RetTime [min]	Type	Area [25 μ V*s]	Amt/Area	Amount [ng/ul]	Grp	Name
3.272		-	-	-		CO2
4.177		-	-	-		N02
5.338		-	-	-		Oxygen
6.396		-	-	-		Nitrogen
8.853		-	-	-		Methane

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

*** End of Report ***