


Sample Name: SAMPLE_20251001-1215PM-ELECDON-GOWN311C

```
=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : Green House Gas GC           Location :    1  (F)
Injection Date  : 10/1/2025 4:54:44 PM
                                           Inj Volume : Manually
Method          : C:\Chem32\2\Methods\Gamma-N20-2.M
Last changed    : 10/1/2025 4:48:35 PM by SYSTEM
                  (modified after loading)
```

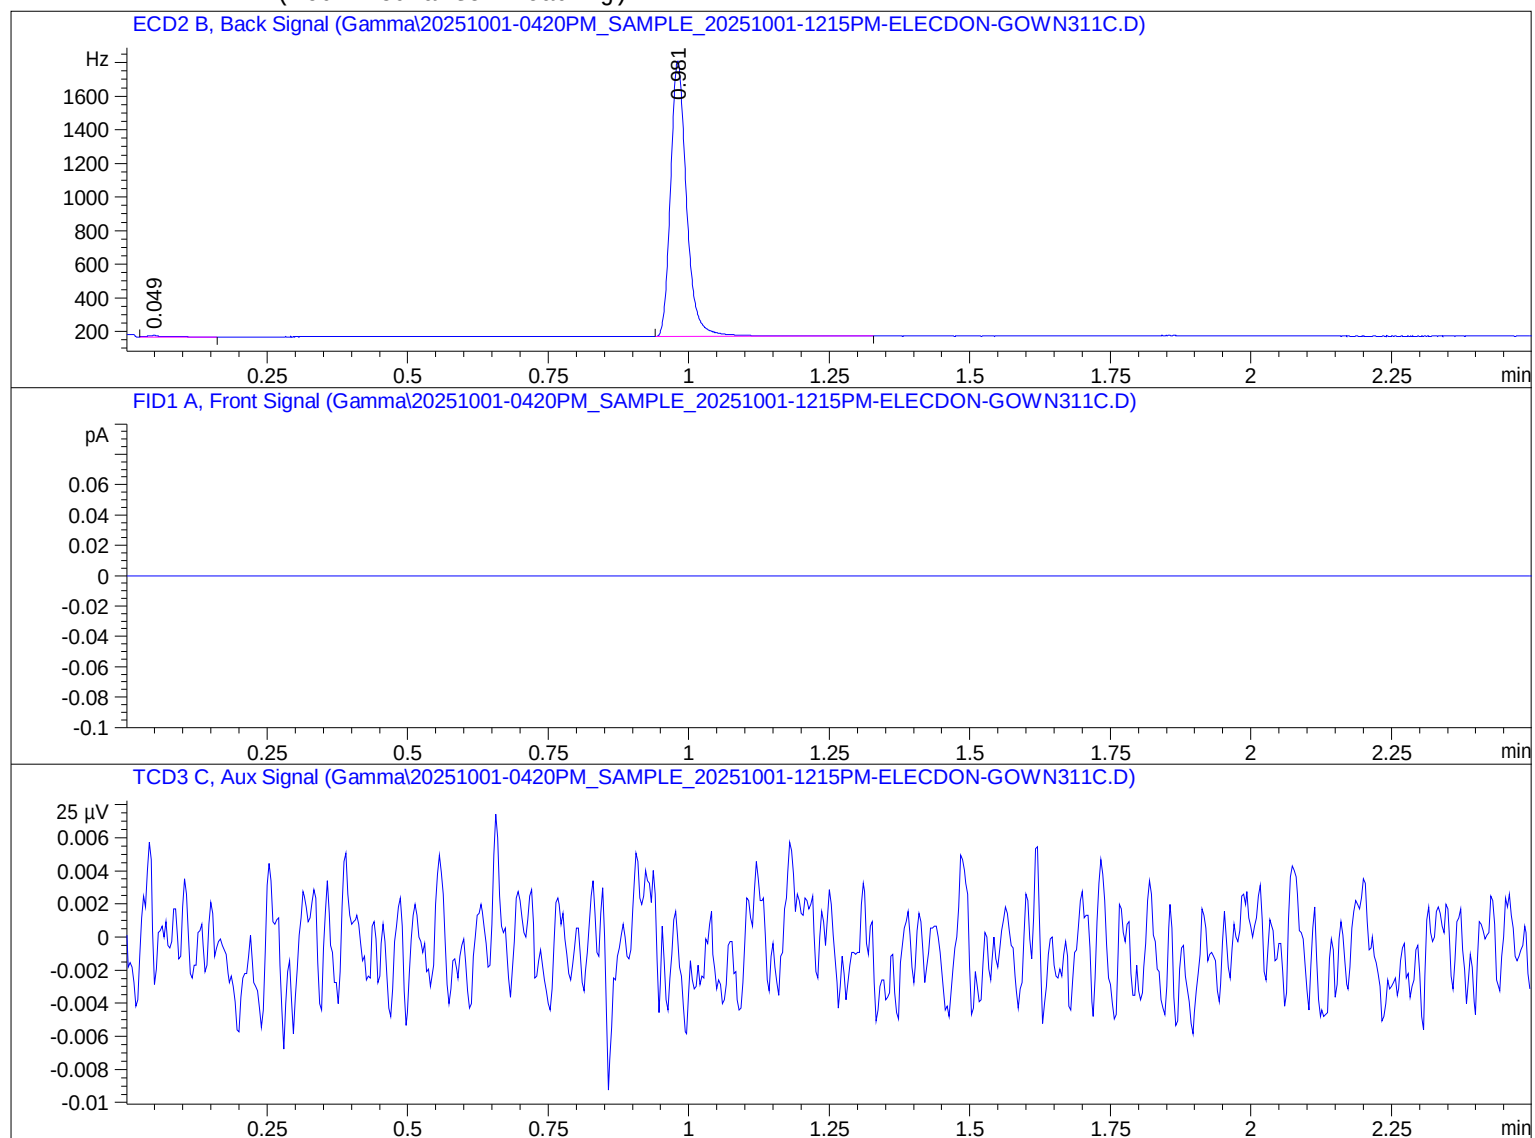

```
=====
External Standard Report
=====
```

```
Sorted By      :      Signal
Calib. Data Modified :    10/1/2025 2:07:40 PM
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Sample Name: SAMPLE_20251001-1215PM-ELECDON-GOWN311C

Signal 1: ECD2 B, Back Signal

RetTime [min]	Type	Area [Hz*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.857		-	-	-		N2O
2.847		-	-	-		N2

Totals : 0.00000

Signal 2: FID1 A, Front Signal

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ng/ul]	Grp	Name
1.141		-	-	-		Methane
1.945		-	-	-		CO2

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

RetTime [min]	Type	Area [25 µV*s]	Amt/Area	Amount [ng/ul]	Grp	Name
3.272		-	-	-		CO2
4.177		-	-	-		N2
5.338		-	-	-		Oxygen
6.396		-	-	-		Nitrogen
8.853		-	-	-		Methane

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====
=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 10/1/2025 2:07:40 PM
Multiplier : 1.0000
Dilution : 1.0000
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: ECD2 B, Back Signal

Peak #	RetTime [min]	Type	Width [min]	Area [Hz*s]	Area %	Name
1	0.049	BB	0.0331	21.61159	0.65747	?
2	0.981	BB	0.0318	3265.49512	99.34253	?
3	1.857		0.0000	0.00000	0.00000	N2O
4	2.847		0.0000	0.00000	0.00000	N02

Totals : 3287.10670

Signal 2: FID1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	1.141		0.0000	0.00000	0.00000	Methane
2	1.945		0.0000	0.00000	0.00000	C02

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

Peak #	RetTime [min]	Type	Width [min]	Area [25 μ V*s]	Area %	Name
1	3.272		0.0000	0.00000	0.00000	C02
2	4.177		0.0000	0.00000	0.00000	N02
3	5.338		0.0000	0.00000	0.00000	Oxygen
4	6.396		0.0000	0.00000	0.00000	Nitrogen
5	8.853		0.0000	0.00000	0.00000	Methane

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

*** End of Report ***