


Sample Name: SAMPLE\_20251001-1215PM-ELECDON-GOWN311B

=====

Acq. Operator : SYSTEM  
Sample Operator : SYSTEM  
Acq. Instrument : Green House Gas GC Location : 1 (F)  
Injection Date : 10/1/2025 9:37:08 PM  
Inj Volume : Manually

Method : C:\Chem32\2\Methods\Gamma-N20-2.M  
Last changed : 10/1/2025 9:35:43 PM by SYSTEM  
(modified after loading)

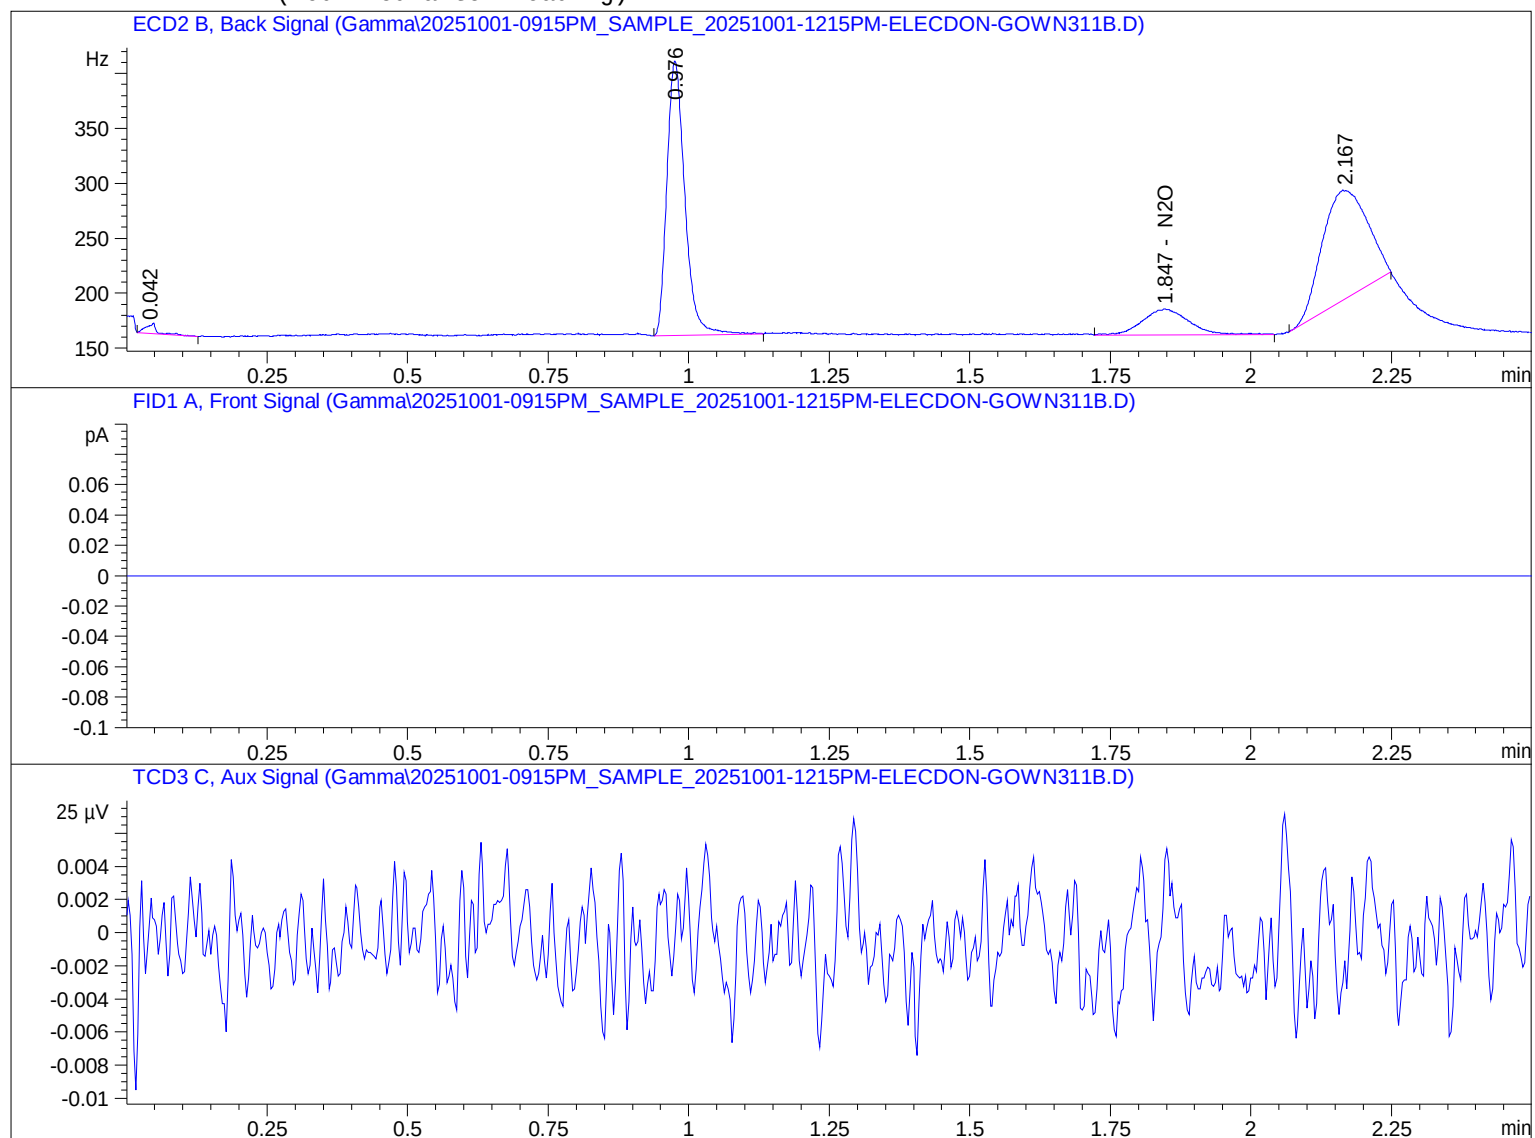

=====

External Standard Report

=====

Sorted By : Signal  
Calib. Data Modified : 10/1/2025 2:07:40 PM  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Sample Name: SAMPLE\_20251001-1215PM-ELECDON-GOWN311B

## Signal 1: ECD2 B, Back Signal

| RetTime<br>[min] | Type | Area<br>[Hz*s] | Amt/Area   | Amount<br>[ng/ul] | Grp | Name |
|------------------|------|----------------|------------|-------------------|-----|------|
| 1.847            | BB   | 132.74411      | 3.11253e-3 | 4.13170e-1        | N20 |      |
| 2.847            |      | -              | -          | -                 | N02 |      |

Totals : 4.13170e-1

## Signal 2: FID1 A, Front Signal

| RetTime<br>[min] | Type | Area<br>[pA*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name    |
|------------------|------|----------------|----------|-------------------|-----|---------|
| 1.141            |      | -              | -        | -                 |     | Methane |
| 1.945            |      | -              | -        | -                 |     | CO2     |

Totals : 0.00000

## Signal 3: TCD3 C, Aux Signal

| RetTime<br>[min] | Type | Area<br>[25 µV*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name     |
|------------------|------|-------------------|----------|-------------------|-----|----------|
| 3.272            |      | -                 | -        | -                 |     | CO2      |
| 4.177            |      | -                 | -        | -                 |     | N02      |
| 5.338            |      | -                 | -        | -                 |     | Oxygen   |
| 6.396            |      | -                 | -        | -                 |     | Nitrogen |
| 8.853            |      | -                 | -        | -                 |     | Methane  |

Totals : 0.00000

## 1 Warnings or Errors :

Warning : Calibrated compound(s) not found

\*\*\* End of Report \*\*\*