


Sample Name: SAMPLE\_20250921-1245PM-D87LIQ-SS1

=====

Acq. Operator : SYSTEM  
Sample Operator : SYSTEM  
Acq. Instrument : Green House Gas GC Location : 1 (F)  
Injection Date : 9/25/2025 6:01:35 PM  
Inj Volume : Manually

Method : C:\Chem32\2\Methods\Gamma-N2O-2.M  
Last changed : 9/25/2025 4:45:02 PM by SYSTEM  
(modified after loading)

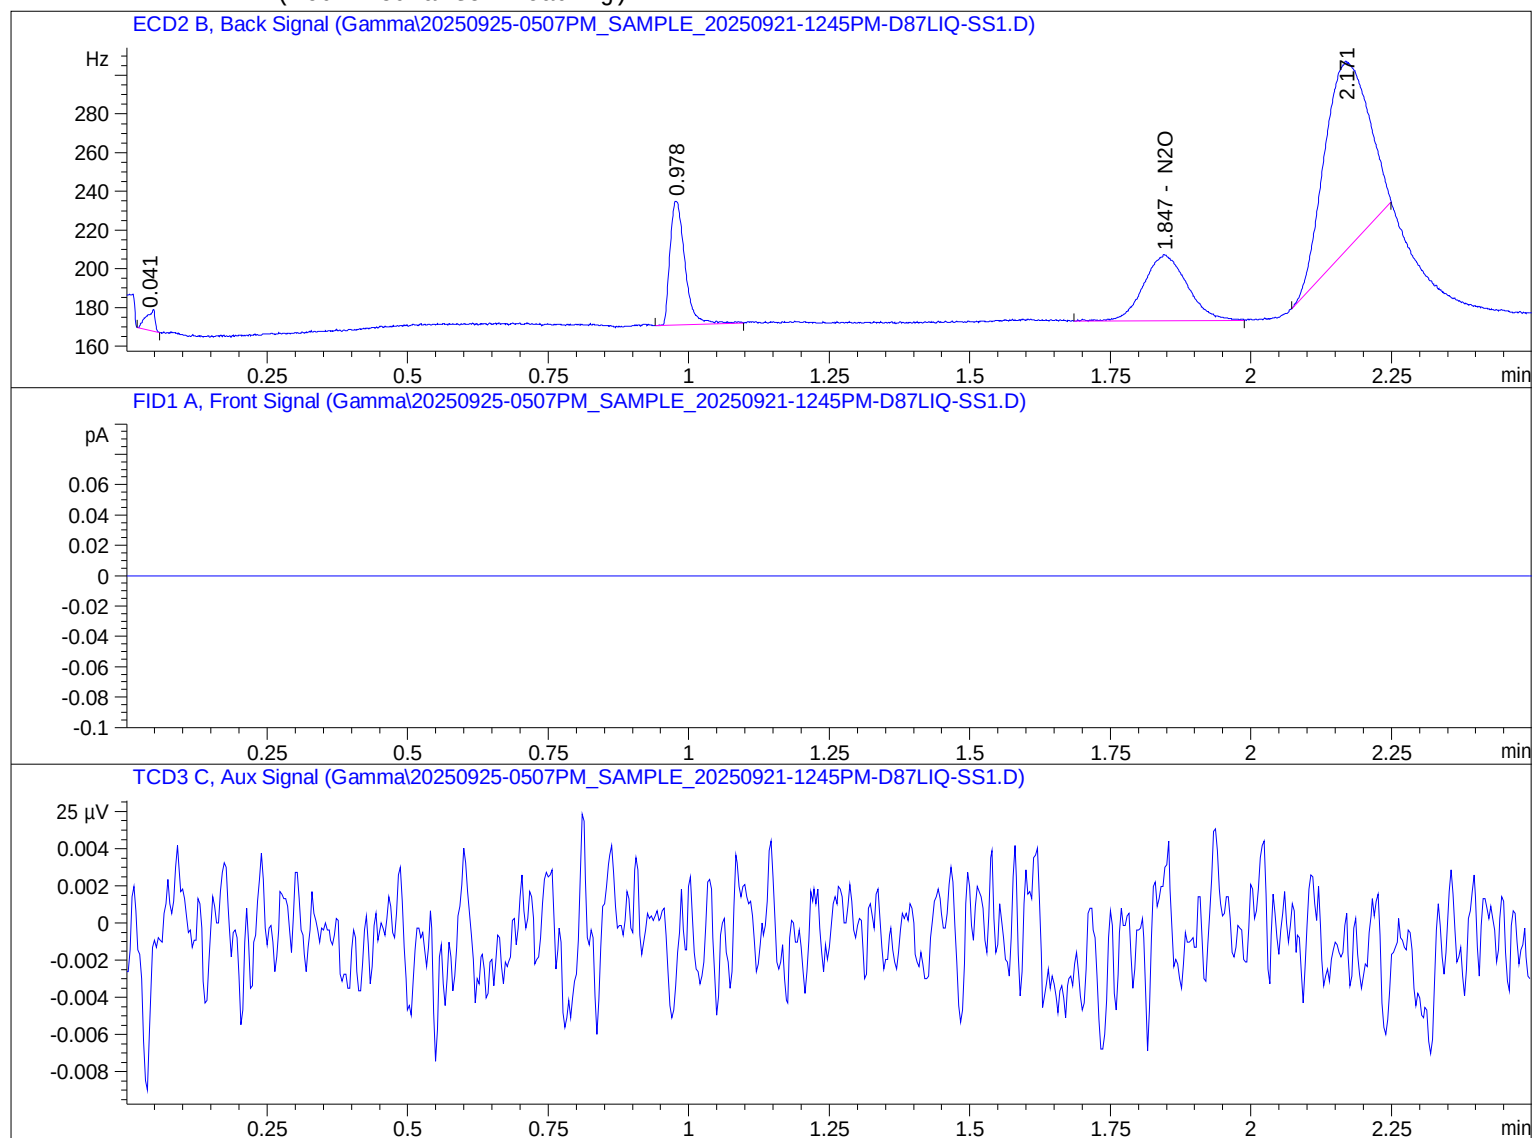

=====  
External Standard Report  
=====

Sorted By : Signal  
Calib. Data Modified : 9/25/2025 2:17:23 PM  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: ECD2 B, Back Signal

| RetTime<br>[min] | Type | Area<br>[Hz*s] | Amt/Area   | Amount<br>[ng/ul] | Grp | Name |
|------------------|------|----------------|------------|-------------------|-----|------|
| 1.847            | BB   | 184.61131      | 3.75039e-3 | 6.92365e-1        | N20 |      |
| 2.847            |      | -              | -          | -                 | N02 |      |

Totals : 6.92365e-1

Signal 2: FID1 A, Front Signal

| RetTime<br>[min] | Type | Area<br>[pA*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name    |
|------------------|------|----------------|----------|-------------------|-----|---------|
| 1.141            |      | -              | -        | -                 |     | Methane |
| 1.945            |      | -              | -        | -                 |     | C02     |

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

| RetTime<br>[min] | Type | Area<br>[25 µV*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name     |
|------------------|------|-------------------|----------|-------------------|-----|----------|
| 3.272            |      | -                 | -        | -                 |     | C02      |
| 4.177            |      | -                 | -        | -                 |     | N02      |
| 5.338            |      | -                 | -        | -                 |     | Oxygen   |
| 6.396            |      | -                 | -        | -                 |     | Nitrogen |
| 8.853            |      | -                 | -        | -                 |     | Methane  |

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====  
\*\*\* End of Report \*\*\*