


Sample Name: SAMPLE\_20250921-1245PM-D87LIQ-SS2

```
=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : Green House Gas GC           Location :    1  (F)
Injection Date  : 9/25/2025 6:05:47 PM
                                           Inj Volume : Manually

Acq. Method     : C:\Chem32\2\Methods\Gammaamma-N20-2.M
Last changed    : 9/25/2025 4:45:02 PM by SYSTEM
                  (modified after loading)
Analysis Method : C:\Chem32\2\Methods\Gammaamma-N20-2.M
Last changed    : 9/25/2025 6:08:39 PM by SYSTEM
                  (modified after loading)
Additional Info  : Peak(s) manually integrated
=====
```

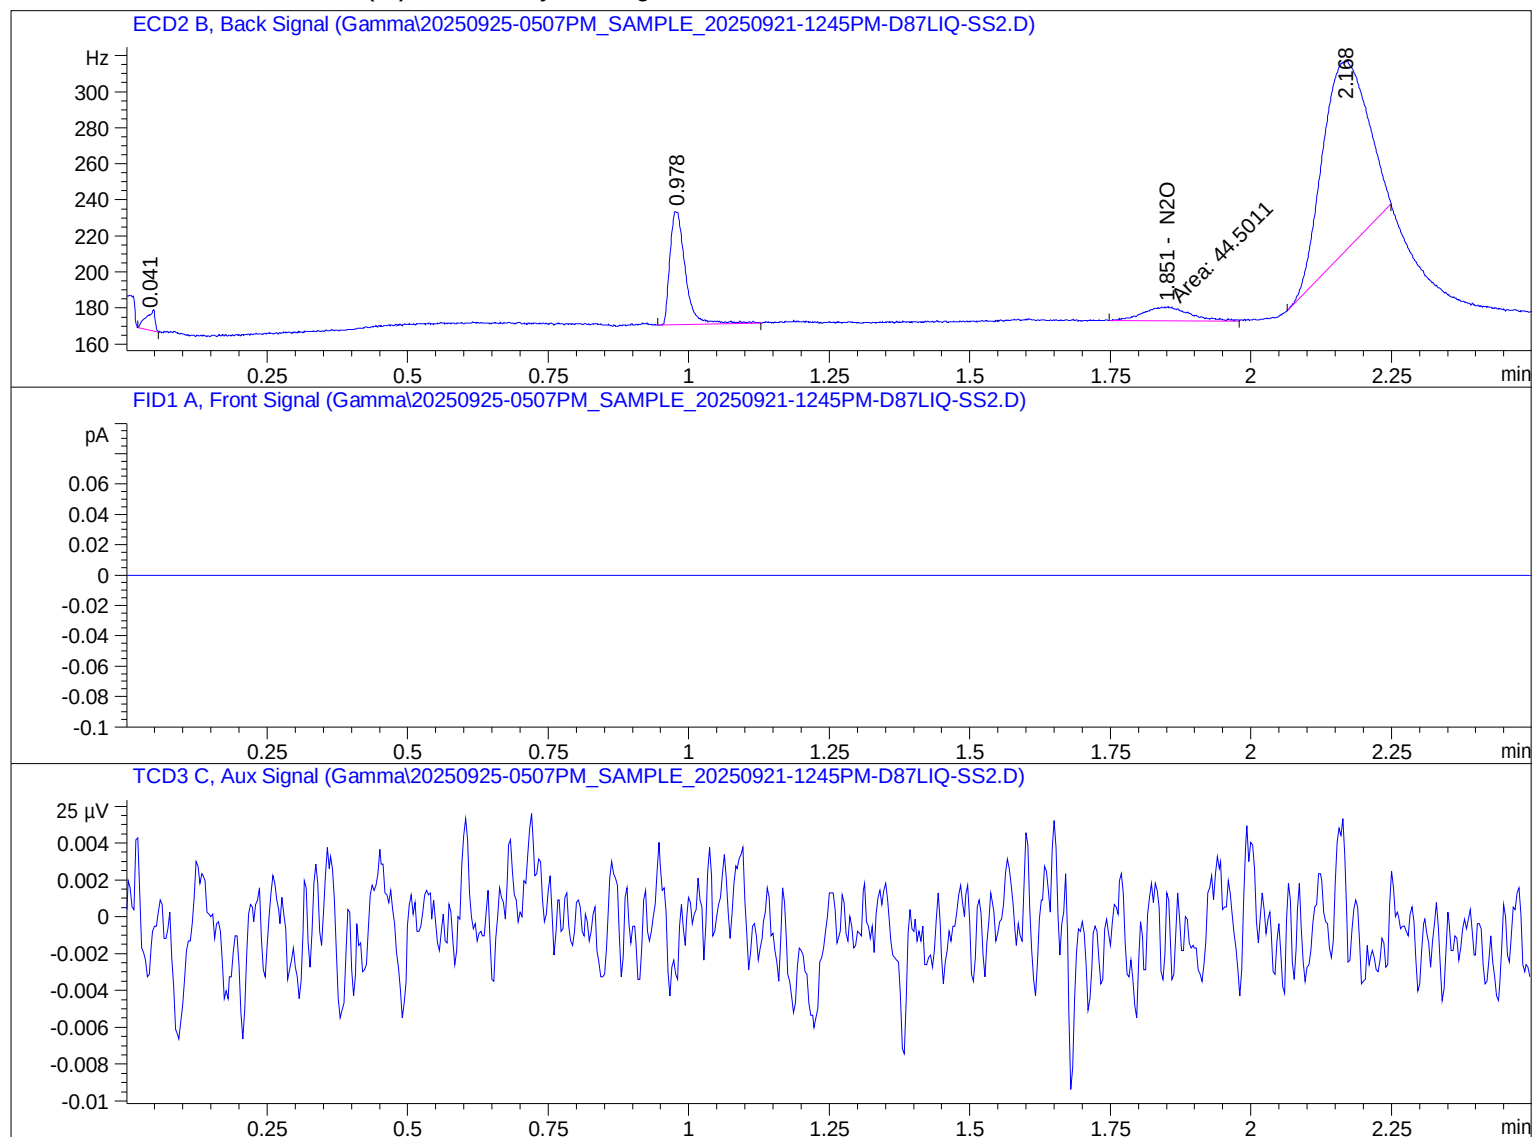

```
=====
External Standard Report
=====
```

```
Sorted By       :      Signal
Calib. Data Modified :    9/25/2025 2:17:23 PM
Multiplier      :    1.0000
Dilution        :    1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: ECD2 B, Back Signal

| RetTime<br>[min] | Type | Area<br>[Hz*s] | Amt/Area   | Amount<br>[ng/ul] | Grp | Name |
|------------------|------|----------------|------------|-------------------|-----|------|
| 1.851            | MM   | 44.50107       | 3.75039e-3 | 1.66897e-1        |     | N2O  |
| 2.847            |      | -              | -          | -                 |     | N02  |

Totals : 1.66897e-1

Signal 2: FID1 A, Front Signal

| RetTime<br>[min] | Type | Area<br>[pA*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name    |
|------------------|------|----------------|----------|-------------------|-----|---------|
| 1.141            |      | -              | -        | -                 |     | Methane |
| 1.945            |      | -              | -        | -                 |     | C02     |

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

| RetTime<br>[min] | Type | Area<br>[25 µV*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name     |
|------------------|------|-------------------|----------|-------------------|-----|----------|
| 3.272            |      | -                 | -        | -                 |     | C02      |
| 4.177            |      | -                 | -        | -                 |     | N02      |
| 5.338            |      | -                 | -        | -                 |     | Oxygen   |
| 6.396            |      | -                 | -        | -                 |     | Nitrogen |
| 8.853            |      | -                 | -        | -                 |     | Methane  |

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====  
\*\*\* End of Report \*\*\*