


Sample Name: SAMPLE\_20250921-1245PM-D87LIQ-CL3

```
=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : Green House Gas GC           Location :    1  (F)
Injection Date  : 9/25/2025 9:26:59 PM
                                           Inj Volume : Manually
Method          : C:\Chem32\2\Methods\Gamma-N2O-2.M
Last changed    : 9/25/2025 9:21:19 PM by SYSTEM
                  (modified after loading)
```

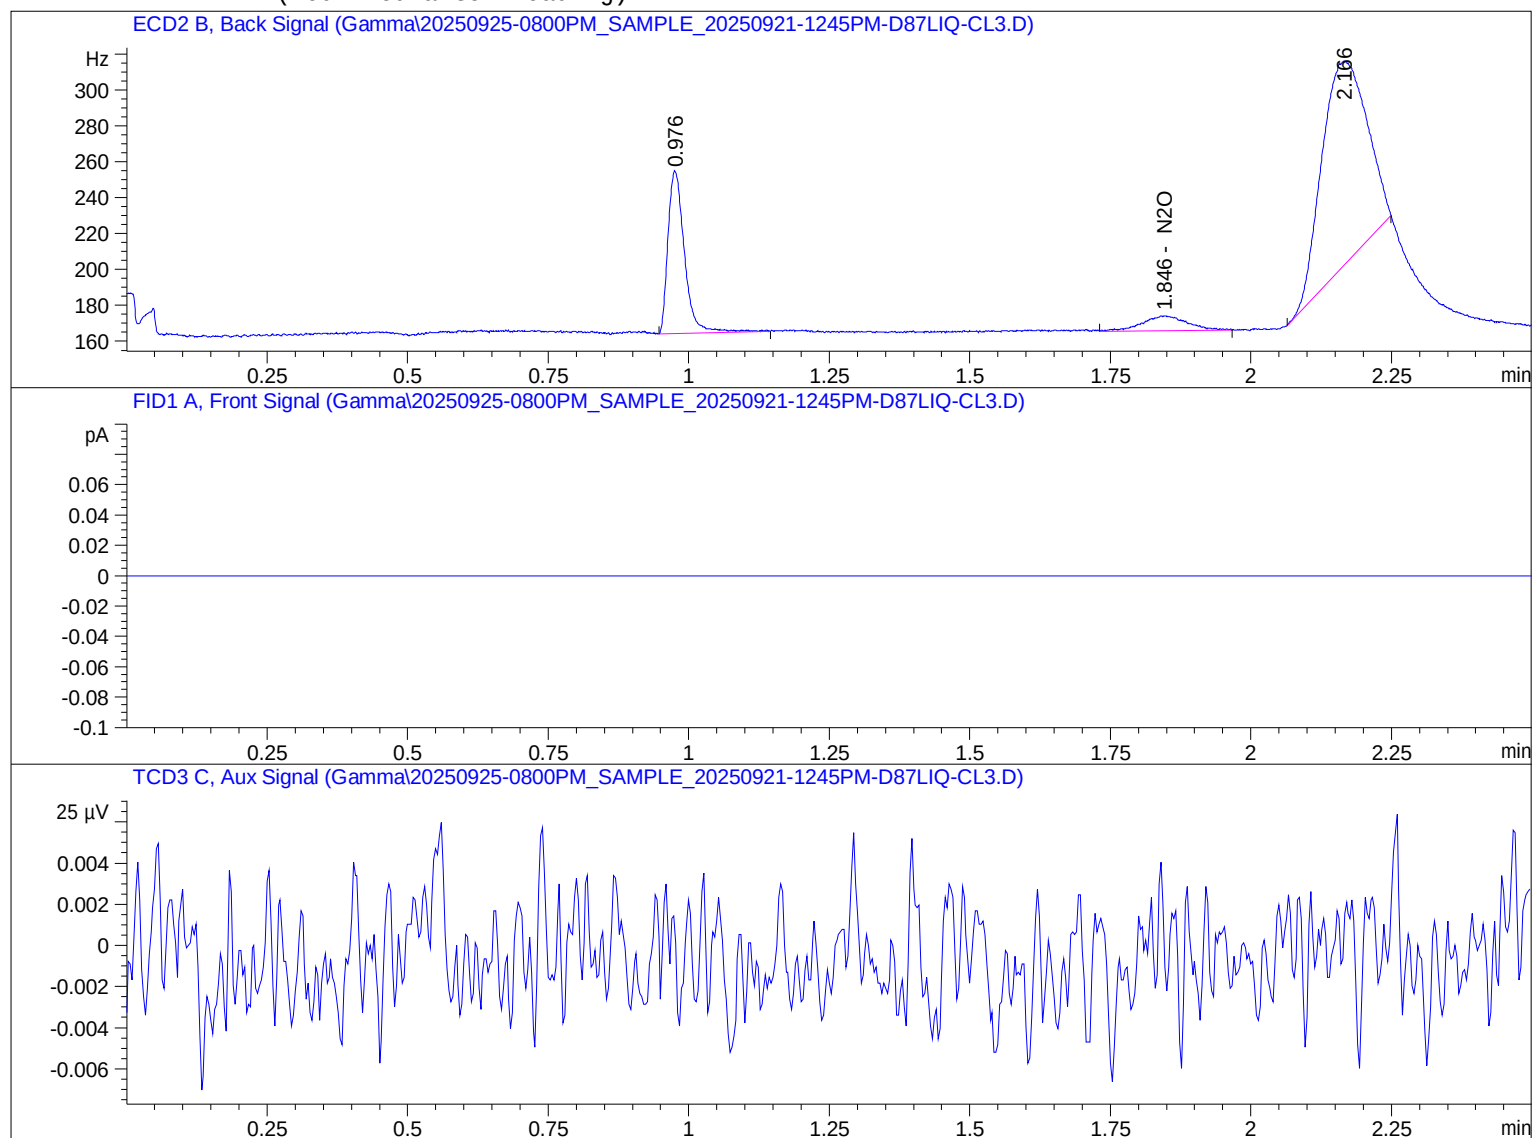

```
=====
External Standard Report
=====
```

```
Sorted By      :      Signal
Calib. Data Modified :      9/25/2025 2:17:23 PM
Multiplier     :      1.0000
Dilution       :      1.0000
```

Do not use Multiplier &amp; Dilution Factor with ISTDs

Signal 1: ECD2 B, Back Signal

| RetTime<br>[min] | Type | Area<br>[Hz*s] | Amt/Area   | Amount<br>[ng/ul] | Grp | Name |
|------------------|------|----------------|------------|-------------------|-----|------|
| 1.846            | BB   | 46.39162       | 3.75039e-3 | 1.73987e-1        | N20 |      |
| 2.847            |      | -              | -          | -                 | N02 |      |

Totals : 1.73987e-1

Signal 2: FID1 A, Front Signal

| RetTime<br>[min] | Type | Area<br>[pA*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name    |
|------------------|------|----------------|----------|-------------------|-----|---------|
| 1.141            |      | -              | -        | -                 |     | Methane |
| 1.945            |      | -              | -        | -                 |     | C02     |

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

| RetTime<br>[min] | Type | Area<br>[25 $\mu$ V*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name     |
|------------------|------|------------------------|----------|-------------------|-----|----------|
| 3.272            |      | -                      | -        | -                 |     | C02      |
| 4.177            |      | -                      | -        | -                 |     | N02      |
| 5.338            |      | -                      | -        | -                 |     | Oxygen   |
| 6.396            |      | -                      | -        | -                 |     | Nitrogen |
| 8.853            |      | -                      | -        | -                 |     | Methane  |

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

\*\*\* End of Report \*\*\*