


Sample Name: Calibration\_N2O-Standards-0ppm-1

```
=====
Acq. Operator   : SYSTEM
Sample Operator : SYSTEM
Acq. Instrument : Green House Gas GC           Location :    1  (F)
Injection Date  : 9/30/2025 1:53:25 PM
                                           Inj Volume : Manually
Method          : C:\Chem32\2\Methods\Gamma-N2O-2.M
Last changed    : 9/30/2025 1:51:16 PM by SYSTEM
                  (modified after loading)
```

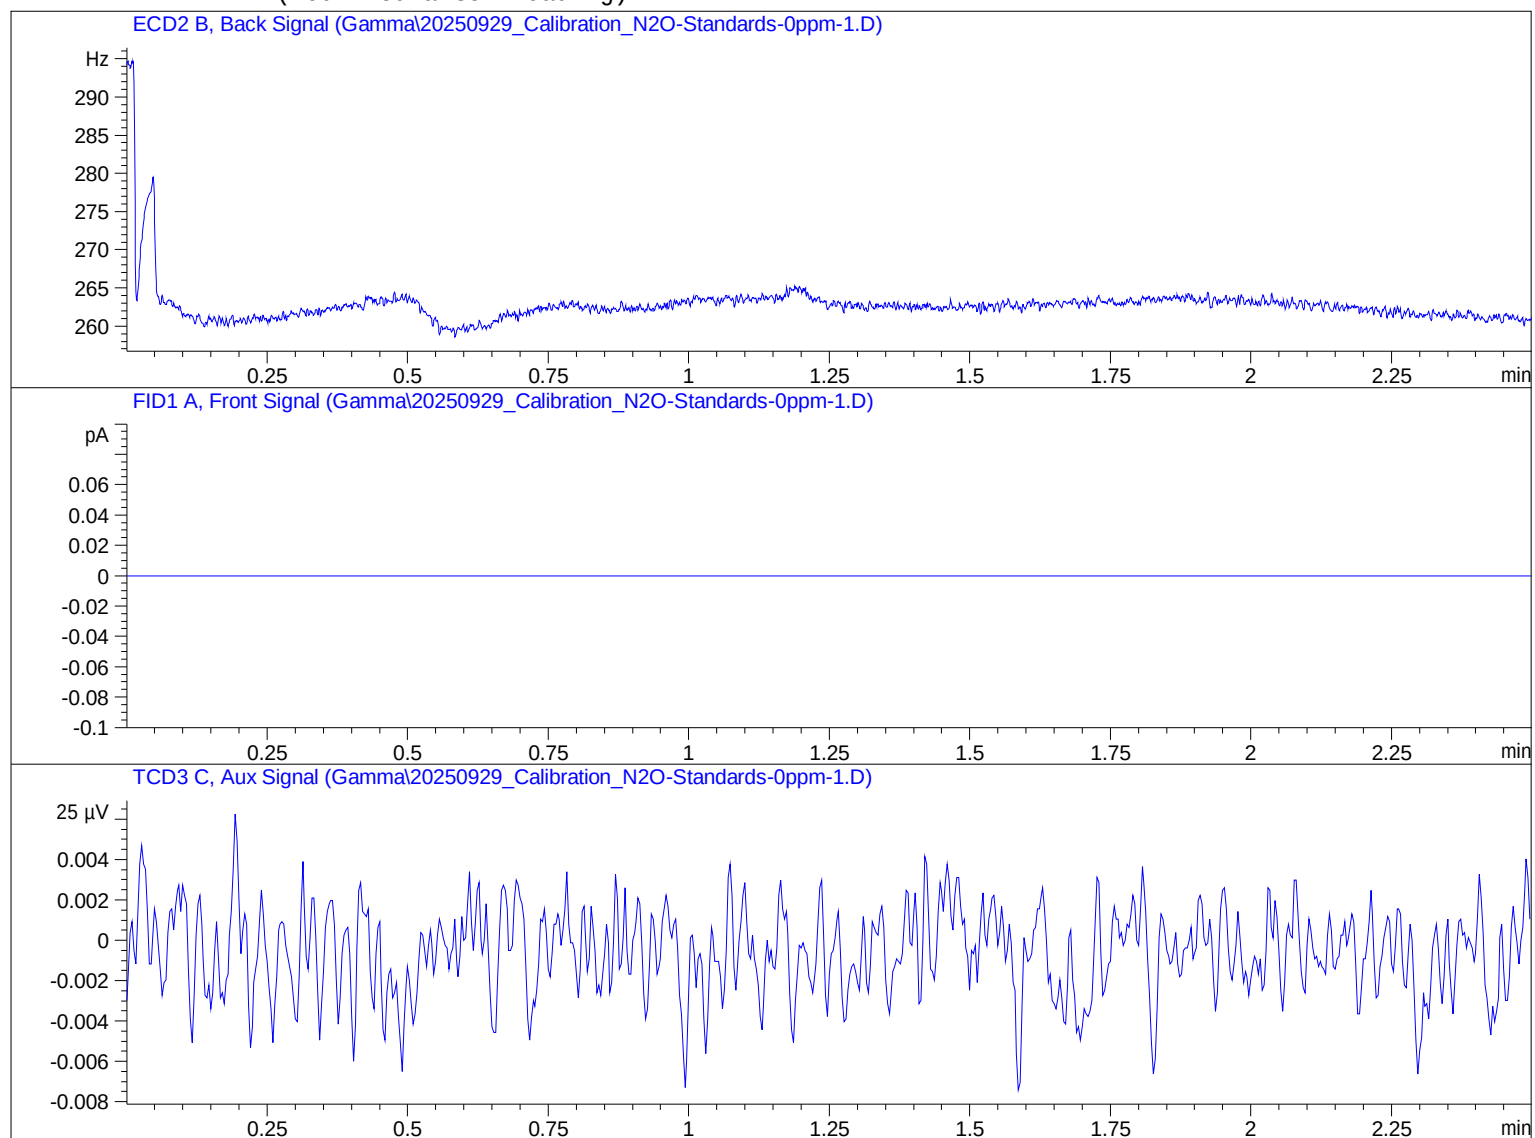

```
=====
External Standard Report
=====
```

```
Sorted By      :      Signal
Calib. Data Modified :      9/30/2025 1:45:24 PM
Multiplier     :      1.0000
Dilution       :      1.0000
Do not use Multiplier & Dilution Factor with ISTDs
```

Signal 1: ECD2 B, Back Signal

| RetTime<br>[min] | Type | Area<br>[Hz*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name |
|------------------|------|----------------|----------|-------------------|-----|------|
| 1.857            |      | -              | -        | -                 |     | N20  |
| 2.847            |      | -              | -        | -                 |     | N02  |

Totals : 0.00000

Signal 2: FID1 A, Front Signal

| RetTime<br>[min] | Type | Area<br>[pA*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name    |
|------------------|------|----------------|----------|-------------------|-----|---------|
| 1.141            |      | -              | -        | -                 |     | Methane |
| 1.945            |      | -              | -        | -                 |     | C02     |

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

| RetTime<br>[min] | Type | Area<br>[25 µV*s] | Amt/Area | Amount<br>[ng/ul] | Grp | Name     |
|------------------|------|-------------------|----------|-------------------|-----|----------|
| 3.272            |      | -                 | -        | -                 |     | C02      |
| 4.177            |      | -                 | -        | -                 |     | N02      |
| 5.338            |      | -                 | -        | -                 |     | Oxygen   |
| 6.396            |      | -                 | -        | -                 |     | Nitrogen |
| 8.853            |      | -                 | -        | -                 |     | Methane  |

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====  
=====  
Area Percent Report  
=====

Sorted By : Signal  
Calib. Data Modified : 9/30/2025 1:45:24 PM  
Multiplier : 1.0000  
Dilution : 1.0000  
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: ECD2 B, Back Signal

| Peak # | RetTime [min] | Type | Width [min] | Area [Hz*s] | Area %  | Name |
|--------|---------------|------|-------------|-------------|---------|------|
| 1      | 1.857         |      | 0.0000      | 0.00000     | 0.00000 | N20  |
| 2      | 2.847         |      | 0.0000      | 0.00000     | 0.00000 | N02  |

Totals : 0.00000

Signal 2: FID1 A, Front Signal

| Peak # | RetTime [min] | Type | Width [min] | Area [pA*s] | Area %  | Name    |
|--------|---------------|------|-------------|-------------|---------|---------|
| 1      | 1.141         |      | 0.0000      | 0.00000     | 0.00000 | Methane |
| 2      | 1.945         |      | 0.0000      | 0.00000     | 0.00000 | C02     |

Totals : 0.00000

Signal 3: TCD3 C, Aux Signal

| Peak # | RetTime [min] | Type | Width [min] | Area [25 µV*s] | Area %  | Name     |
|--------|---------------|------|-------------|----------------|---------|----------|
| 1      | 3.272         |      | 0.0000      | 0.00000        | 0.00000 | C02      |
| 2      | 4.177         |      | 0.0000      | 0.00000        | 0.00000 | N02      |
| 3      | 5.338         |      | 0.0000      | 0.00000        | 0.00000 | Oxygen   |
| 4      | 6.396         |      | 0.0000      | 0.00000        | 0.00000 | Nitrogen |
| 5      | 8.853         |      | 0.0000      | 0.00000        | 0.00000 | Methane  |

Totals : 0.00000

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

\*\*\* End of Report \*\*\*