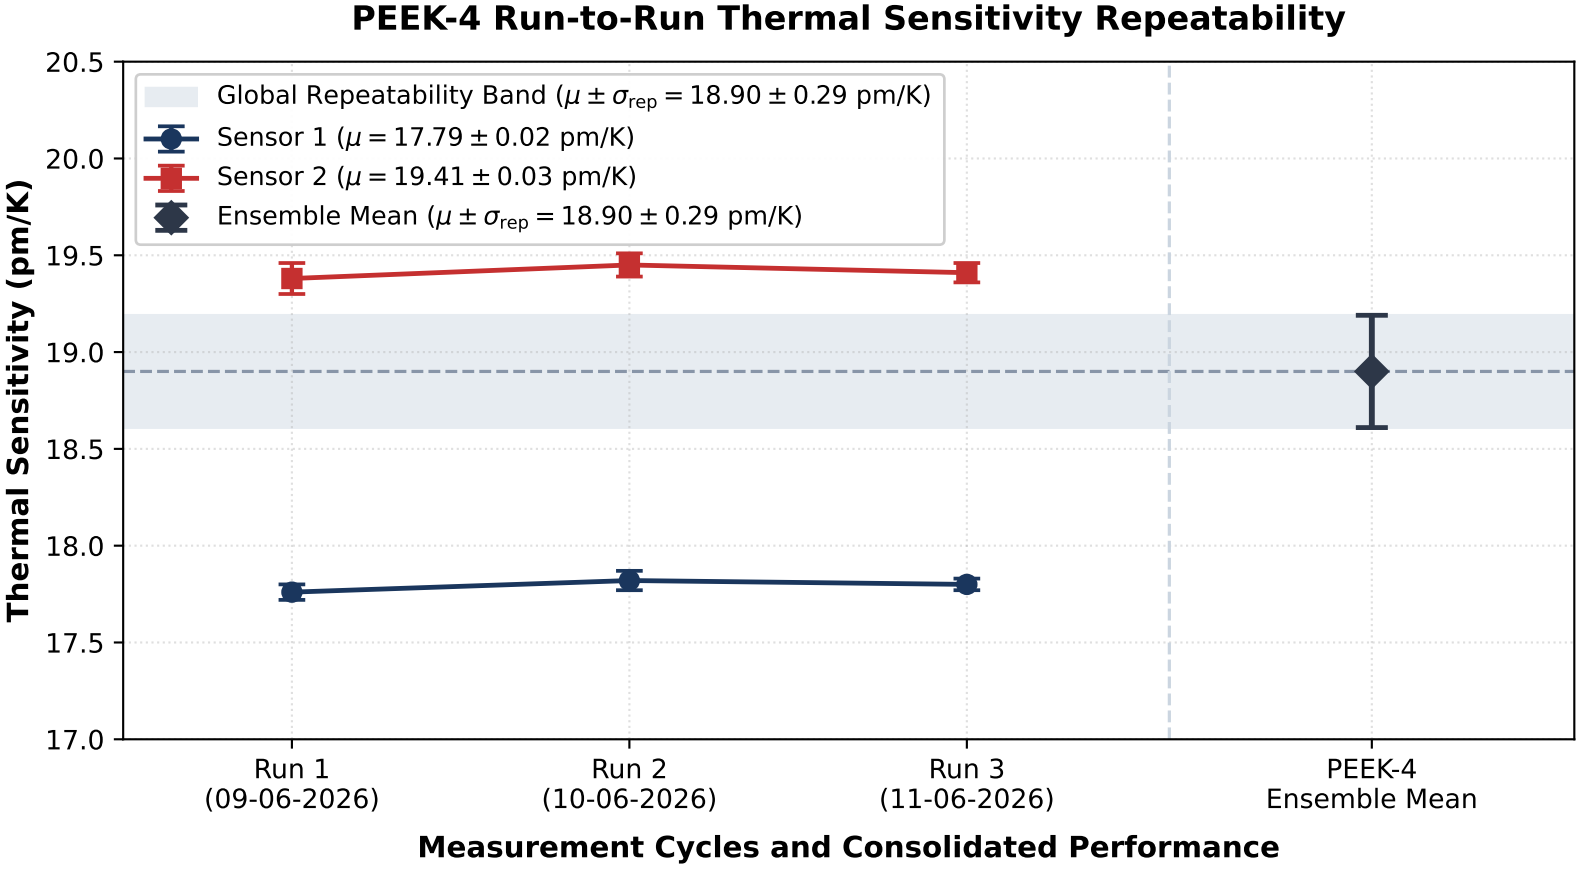
PEEK-4 Run-to-Run Thermal Sensitivity Repeatability
Global Repeatability Band ($\mu \pm \sigma_{rep} = 18.90 \pm 0.29$ pm/K)
Sensor 1 ($\mu = 17.79 \pm 0.02$ pm/K)
Sensor 2 ($\mu = 19.41 \pm 0.03$ pm/K)
Ensemble Mean ($\mu \pm \sigma_{rep} = 18.90 \pm 0.29$ pm/K)
Thermal Sensitivity (pm/K)
20.5
20.0
19.5
19.0
18.5
18.0
17.5
17.0
Run 1
(09-06-2026)
Run 2
(10-06-2026)
Run 3
(11-06-2026)
PEEK-4
Ensemble Mean
Measurement Cycles and Consolidated Performance