


Donat & Mueller 2025: normalized TGA observations
Interval F1 diagnostic uses approximate source capacity 0.77 g/g; no fitted kinetics

dry



humid unlabeled

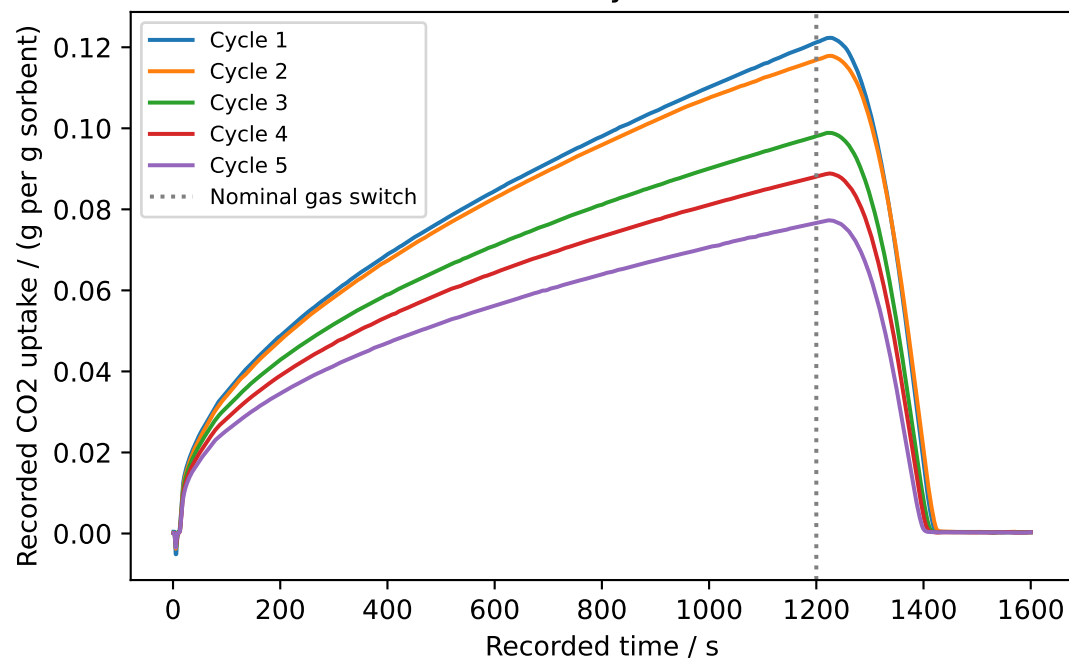