

KN/CAL	/CDE/01			
Issue 04/2020 (01)				
Revision	00			
Page	Page <b>1</b> of <b>10</b>			

#### **AUTHORIZATION:**

This document is issued under the following authority:

ROLE	NAME	DESIGNATION	SIGNATURE	DATE
ISSUE	DANCAN O.	QA TECHNICIAN		2020-04-21
APPROVE	SAMUEL N.	QC SUPERVISOR		

DOCUMENT CONTROL :				
COPY NO	ISSUED TO	ISSUE DATE	REVIEW DATE	
		2020 – –	202 – 0–	
CONTROLL STATUS	CONTROLLED			

#### **TABLE OF CONTENTS**

SR	CONTENT	PAGE NUMBER
I	Records of Changes	3 of 10
II	Distribution/Circulation	3 of 10
III	Abbreviations	4 of 10
1.	Purpose	4 of 10
2.	Scope	4 of 10
3.	References	4 of 10
4.	Principal Responsibilities	5 of 10
5.	Procedure	5 of 10
6.	Appendices	8 of 10



KN/CAL/CDE/01		
Issue	04/2020 (01)	
Revision	00	
Page	Page 2 of 10	

#### I. Records of change

No.	Data	Details of	of Changes Clause/sub-clause and comment	Authorization	
NO.	Date	Page	Clause/sub-clause and comment	Name and Signature	

#### II Distribution/Circulation

Distribution of Controlled copies of this Operating Procedure is as shown below:

1) Copy number 01 - Calibration Technicians

2) Copy number 02 - Calibration team leader

3) Copy number 03 - QC Supervisor

#### III Abbreviations Used

KN - Koko Networks QC - Quality Control

SOP - Standard Operating Procedure

KS - Kenya Standard

ISO - International Organization of Standardisation IEC - International Electrotechnical Committee

CAL - Calibration

CDE - Calibration Data Entry



/CDE/01
04/2020 (01)
00
Page <b>3</b> of <b>10</b>

#### 1. Purpose

This procedure describes the process that ensures the calibration datasheets records can be tracked and have the solution of the following challenges as far as Calibration Reports preparation is concerned. Below are the challenges

- a) Missing Data sheets by the calibration technicians
- b) Misplaced submitted datasheets at the data entry desk
- c) Minimize Wastage of Printing hard papers
- d) Data storage bulkiness (Having huge files of Datasheets, problematic when searching for a datasheet)
- e) Calibration equipment maintenance
- f) Calibration Technicians deviating from calibration procedures

#### 2. SCOPE

This Application procedure applies to both field work and in house calibration activities. It is limited to only Collecting Calibration data as datasheets, but not Verifications or Validations.

#### 3. REFERENCES

- 3.1. KS ISO/IEC 17025:2005: General requirements for the competence of Calibration and testing Laboratories
- 3.2 A-4/07, Traceability of measuring and test equipment to National Standards (previously EAL-G12)
- 3.3 EA-4/11, Calibration and maintenance of measuring and test equipment in testing laboratories, 1996.
- 3.4 NIS 37, A guide to managing the configuration of computer systems (Hardware, software and firmware).
- 3.5 EA/GA (98) 95, Guidelines for the use of computers and computer systems in accredited laboratories

#### 4. **DEFINITIONS**

- 4.1 **Calibration -** The set of operations which establish, under specified conditions, the relationship between values indicated by a measuring instrument or measuring system and Corresponding known values. The results of a calibration permit the estimation of errors associated with the measurement equipment
- 4.2 **Calibration Verification -** Provides a means of determining that deviations between measured values and known values are within the limits of error defined during calibration. The results provide an indication that the instrument/system is working properly.
- 4.3 **Critical Laboratory Equipment** Analytical instrumentation and equipment affecting the accuracy or precision of a test method.
- 4.4 **Performance Verification** The confirmation of the reliability of a previously validated method(s) or equipment.
- 4.5 **Preventive maintenance** program of routine actions such as cleaning, lubrication, adjusting, or testing to keep equipment ready for use. The most important effect of a preventative maintenance program is to ensure measurement system reliability.




KN/CAL/CDI	E/01			
Issue 04/2020 (01)				
Revision	00			
Page	Page <b>4</b> of <b>10</b>			

- 4.6 **Quality Control Checks** Periodic confirmation of the reliability of equipment and instrumentation
- 4.7 Out-of-tolerance A condition in which a measured value of a measurement attribute lies outside the documented performance specifications for the attribute or a state in which one or more attributes of an item are not in conformance with documented performance specifications.
- 5 Principal Responsibilities
- 5.1 The Calibration team leader is responsible for ensuring that the objectives of this procedure are implemented.
- 5.2 The Calibration team leader is responsible for ensuring that the application is used in accordance with set guidance of calibration
- 5.3 All staff conducting Calibration are responsible for ensuring that data entry is done in accordance to this procedure.

#### 6.0 Use of Calibration Data Entry Application Procedure

**6.1** In your internet browser, browse this link <a href="https://gcalibration.github.io/KOKO">https://gcalibration.github.io/KOKO</a> then click the top right menu and Add to Home screen

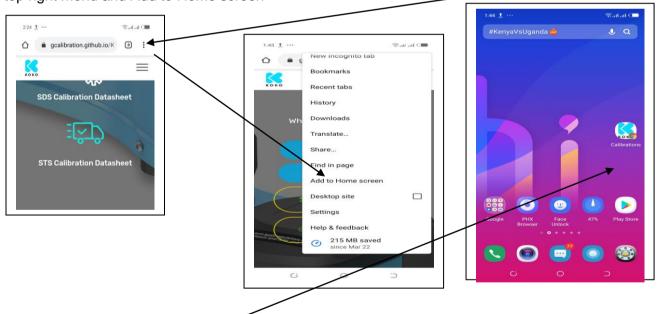


When you check your Home Screen in your phone you will see calibration icon above




KN/CAL/CDE	/01
Issue	04/2020 (01)
Revision	00
Page	Page <b>5</b> of <b>10</b>

6.2 Then click the calibration icon. You will see this page below. This is the home page of the application.

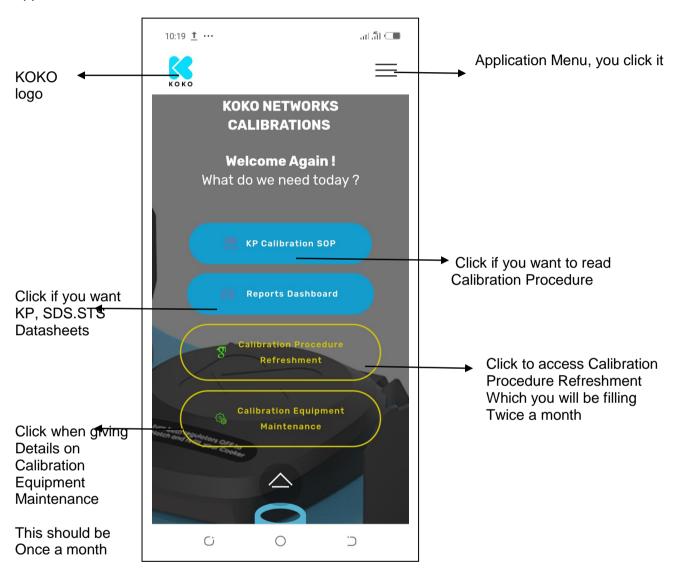


#### 6.3 When you tap Application Menu

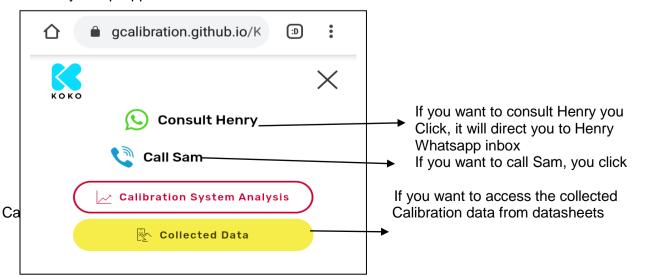




KN/CAL/CDE/01			
Issue	04/2020 (01)		
Revision	00		
Page	Page <b>6</b> of <b>10</b>		

6.4 When you click KP calibration SOP you will see below, when you swipe the screen you go next page

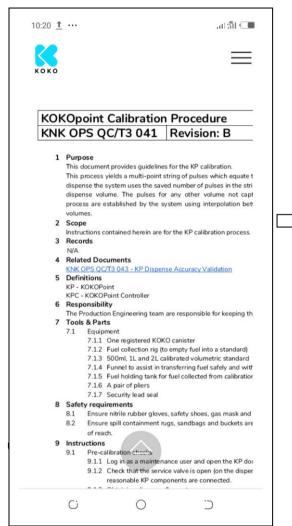

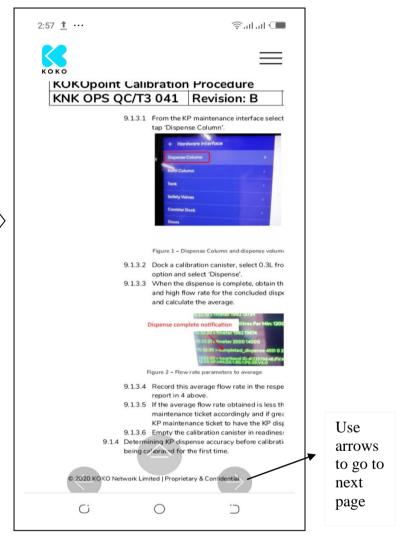

6.5 When you click Report Dashboard you will see 1. Calibration reports in numbers at a glance 2. Reasons for Re-calibration in numbers. Reports are updated automatically every day.

J K	I	Н	G	F	E	D	С	3
CAUSES OF KP RE-CALIBRAT								
4/20/2020				S	ON DUE DATES	(P CALIBRATIO	к	
After Replacing Fuel hose pip	0				2020	4/20/		
After Replacing Pump	0					TED KPs	CALIBRAT	650
After Replacing flow meter	1			TOTAL KPs Due For Recalibration			45	
After Replacing dock assemb	7		130 1-30 Days Out to be Due for Recalibration				130	
After Replacing dispense tray	1		209 31-60 Days Out to be Due for Recalibration					
After Internal Verification	14		ation	r Recalibr	oe Due fo	ys Out to b	61-90 Day	61
After Decomissioned	1		on	≀ecalibrati	Due for F	Out to be	>90 Days	430
During W&M verification	28							
During 3months SG verificati	29							
After 6 months of initial Calib	0							



KN/CAI	L/CDE/01			
Issue 04/2020 (01)				
Revision	00			
Page	Page <b>7</b> of <b>10</b>			

6.6 If you scroll down the home menu






KN/CAL/CDE/01	
Issue	04/2020 (01)
Revision	00
Page	Page <b>8</b> of <b>10</b>

7.0 This application is accordance to ISO 17025 Electronic Data entry/ protection, where the calibration data is controlled and only authorized calibration technician can access the datasheets


As shown when you click KP calibration datasheet icon you see this window where you must log in first

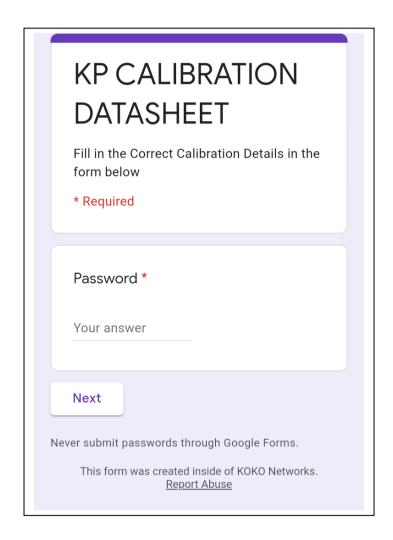



KN/CAL/CDE/01	
Issue	04/2020 (01)
Revision	00
Page	Page <b>9</b> of <b>10</b>

7.1 The Application is subjective to Annual Review and it can be revised as many times as possible for it to comply with the necessary standards

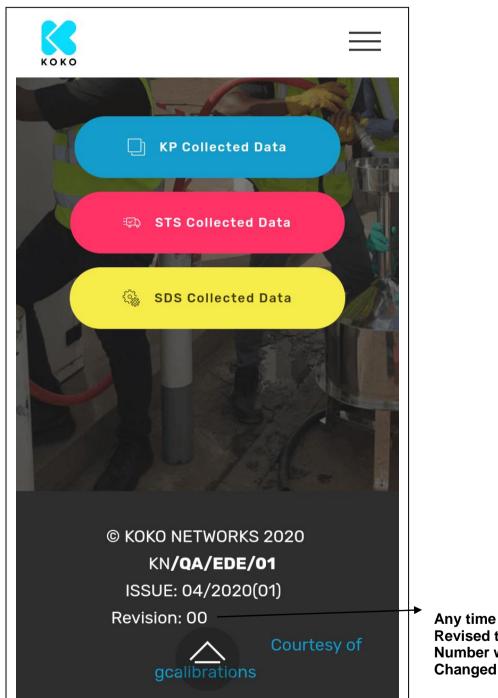

Any time it is **Revised this** Number will be



KN/CAL/CDE/01	
Issue	04/2020 (01)
Revision	00
Page	Page <b>10</b> of <b>10</b>