

IR Dark 0 Og. Pol | Cross-Polarized IR

Measurement report - 63 windows analyzed (10 s, 1 s step) - window is bad if > 30% of its beats fail

1. Measurement condition

Day / experiment	Day 4 / Exp 2 & 3	Polarization channel	Cross-Polarized
Skin tone	Dark	Polarization setup	Og. Pol
Vessel depth	3.5mm	Device orientation	0 deg
Flow speed	Intermediate	Clamp / phantom	Yes / Multilayered
BPM (labeled / measured)	90 / 107	Hardware channel	C21
Phantom wavelength	IR (940 nm)	Recording	2025-10-24T17-02-31 (trial 1, 73 s)
LED channel	IR (940 nm)		

2. Perfusion index



15.65 %

mean $\pm$ 0.08 % SD (across windows)




median 15.66 % range 15.41 - 15.81 %

Window PI = median of its beat PIs
(raw signal, AC/DC x 100, DC = beat trough)

3. Bad window rate

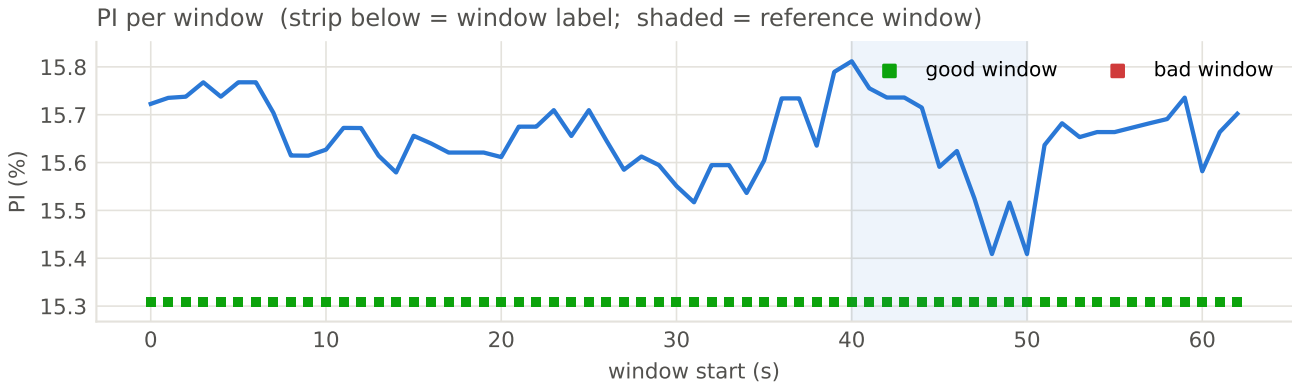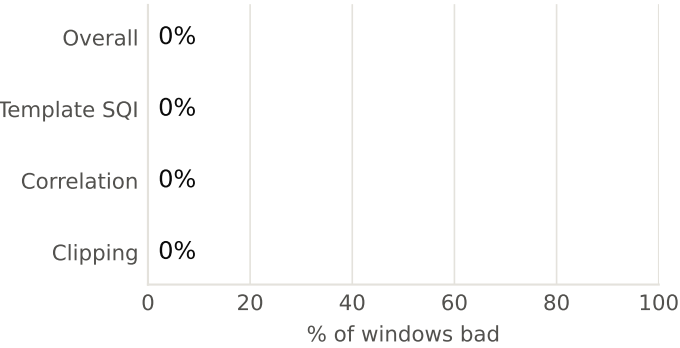

4. Reference window: raw

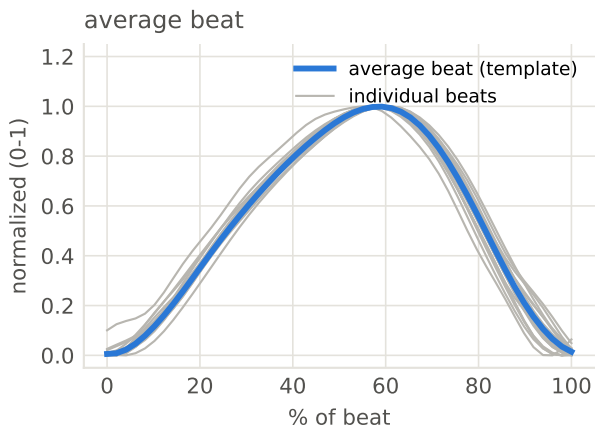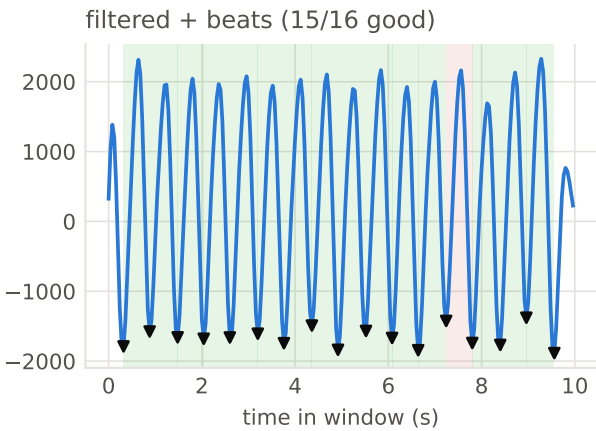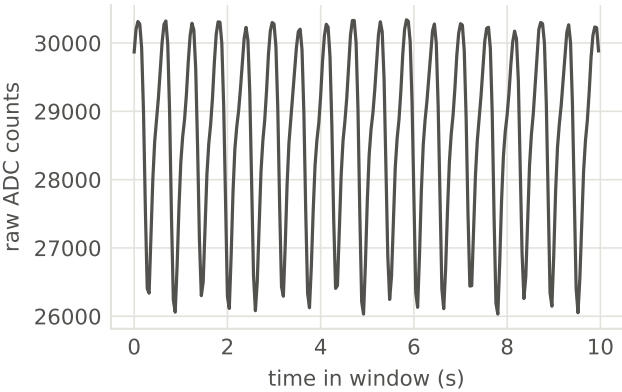

Reference window: 40-50 s (typical good window; labeled good window). A beat fails if template SQI < 0.05, correlation < 0.8, or clipping SQI < 0.8.

Source: 2025-10-24T17-02-31-bc8f07af-eb5d-410e-b237-e4c04fc4cd3f.json