




2021-04-02 DM glucose glycerol acetate calibration 0.1mM

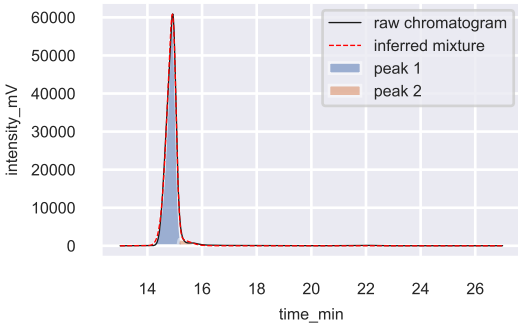


2021-04-02 DM glucose glycerol acetate calibration 0.3mM

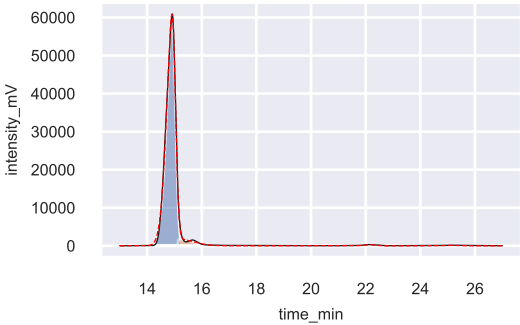


2021-04-02 DM glucose glycerol acetate calibration 0.5mM

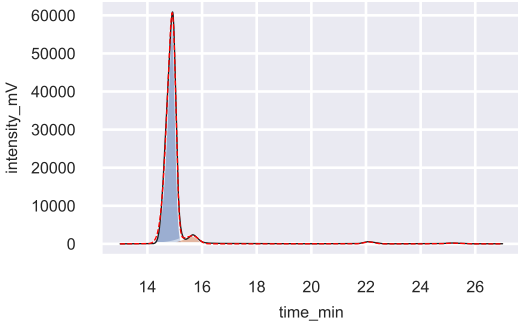


2021-04-02 DM glucose glycerol acetate calibration 01mM

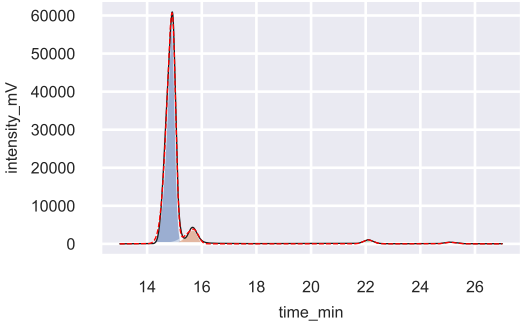


2021-04-02 DM glucose glycerol acetate calibration 02mM

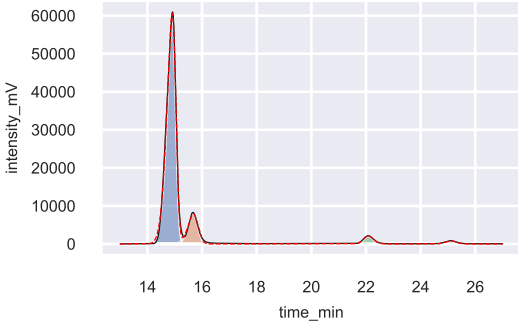


2021-04-02 DM glucose glycerol acetate calibration 03mM

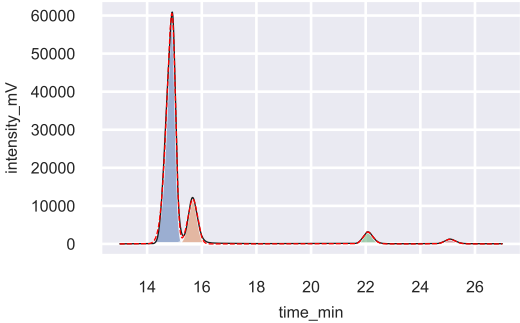


2021-04-02 DM glucose glycerol acetate calibration 05mM

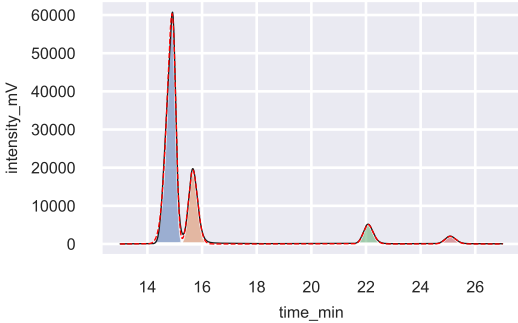


2021-04-02 DM glucose glycerol acetate calibration 0mM

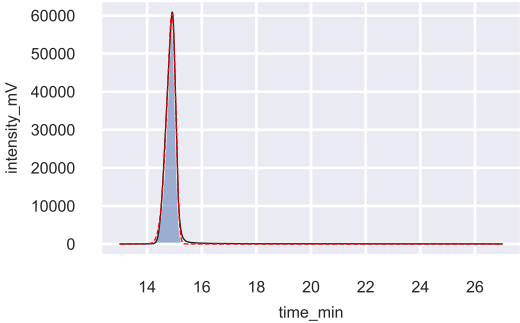


2021-04-02 DM glucose glycerol acetate calibration 10mM

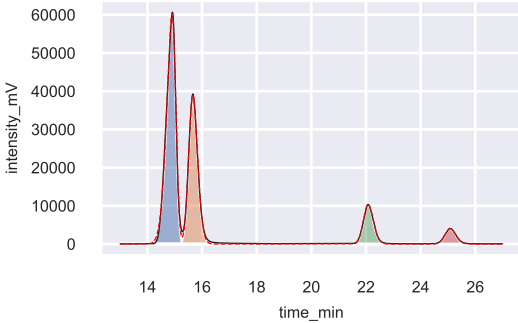


2021-04-02 DM glucose glycerol acetate calibration 15mM

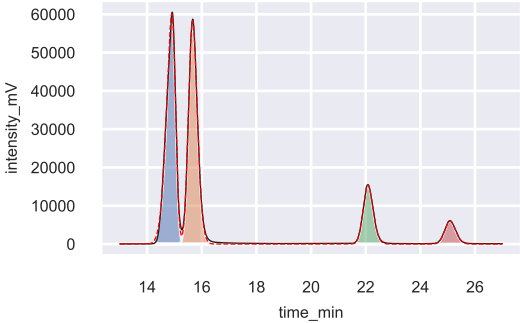

2021-04-02 DM glucose glycerol acetate calibration 20mM

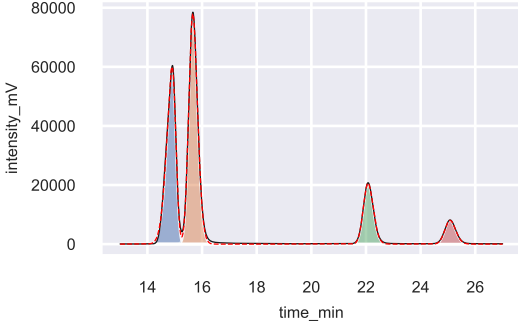

2021-04-02 DM glucose glycerol acetate calibration 25mM

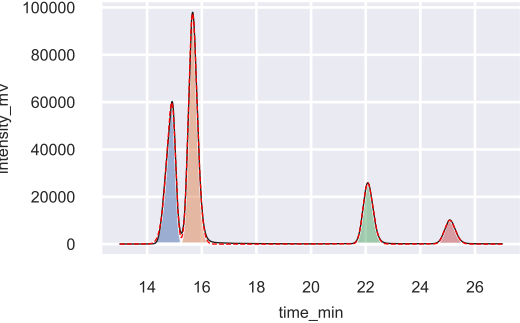

2021-04-02 DM glucose glycerol acetate calibration 30mM

