




2021-04-02 NC glucose glycerol acetate calibration 0.25mM

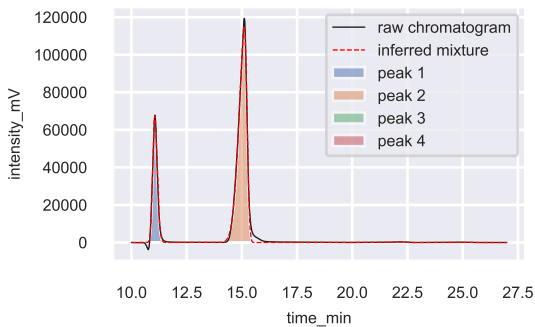


2021-04-02 NC glucose glycerol acetate calibration 00mM

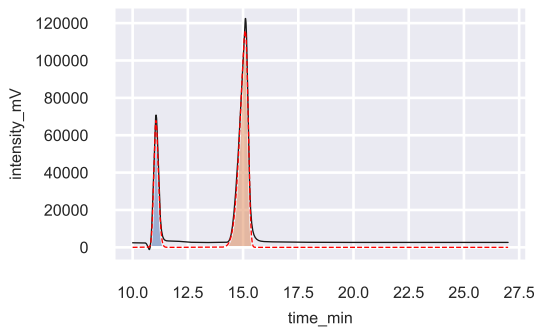


2021-04-02 NC glucose glycerol acetate calibration 01mM

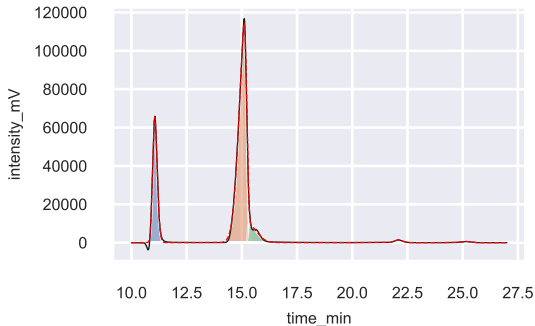


2021-04-02 NC glucose glycerol acetate calibration 02mM

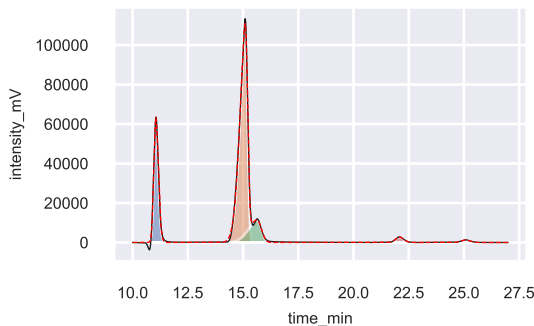


2021-04-02 NC glucose glycerol acetate calibration 03mM

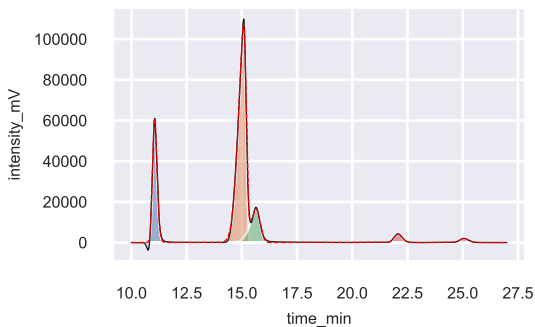


2021-04-02 NC glucose glycerol acetate calibration 05mM

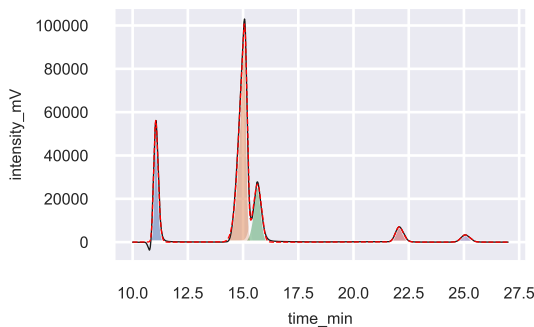


2021-04-02 NC glucose glycerol acetate calibration 10mM

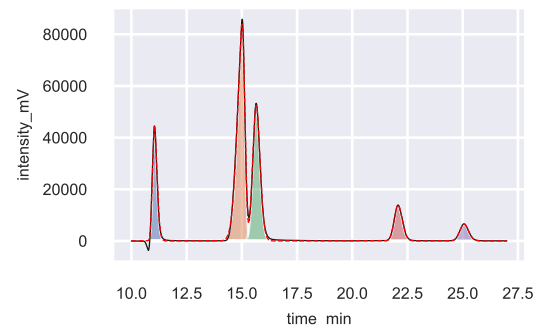


2021-04-02 NC glucose glycerol acetate calibration 15mM

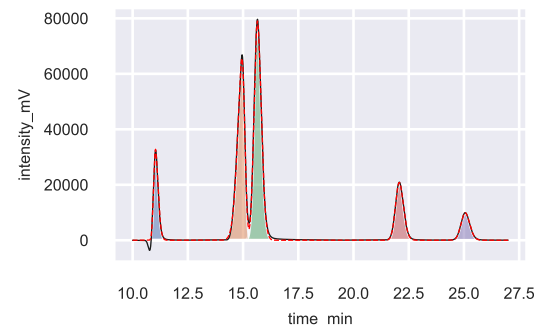

2021-04-02 NC glucose glycerol acetate calibration 20mM

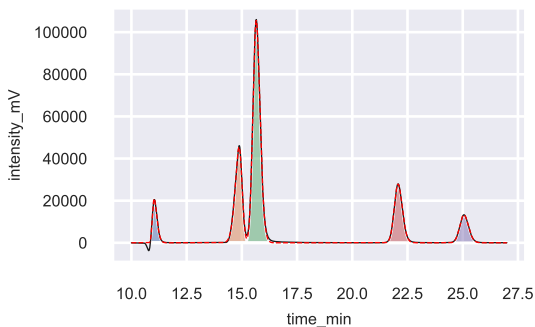

2021-04-02 NC glucose glycerol acetate calibration 25mM

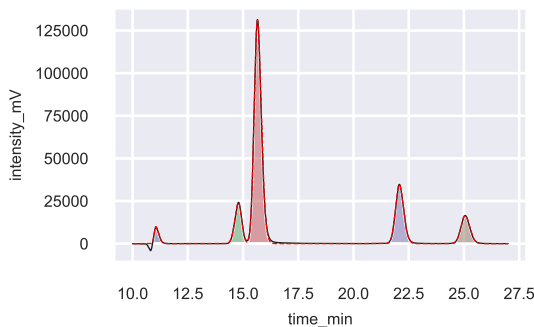

2021-04-02 NC glucose glycerol acetate calibration 30mM

