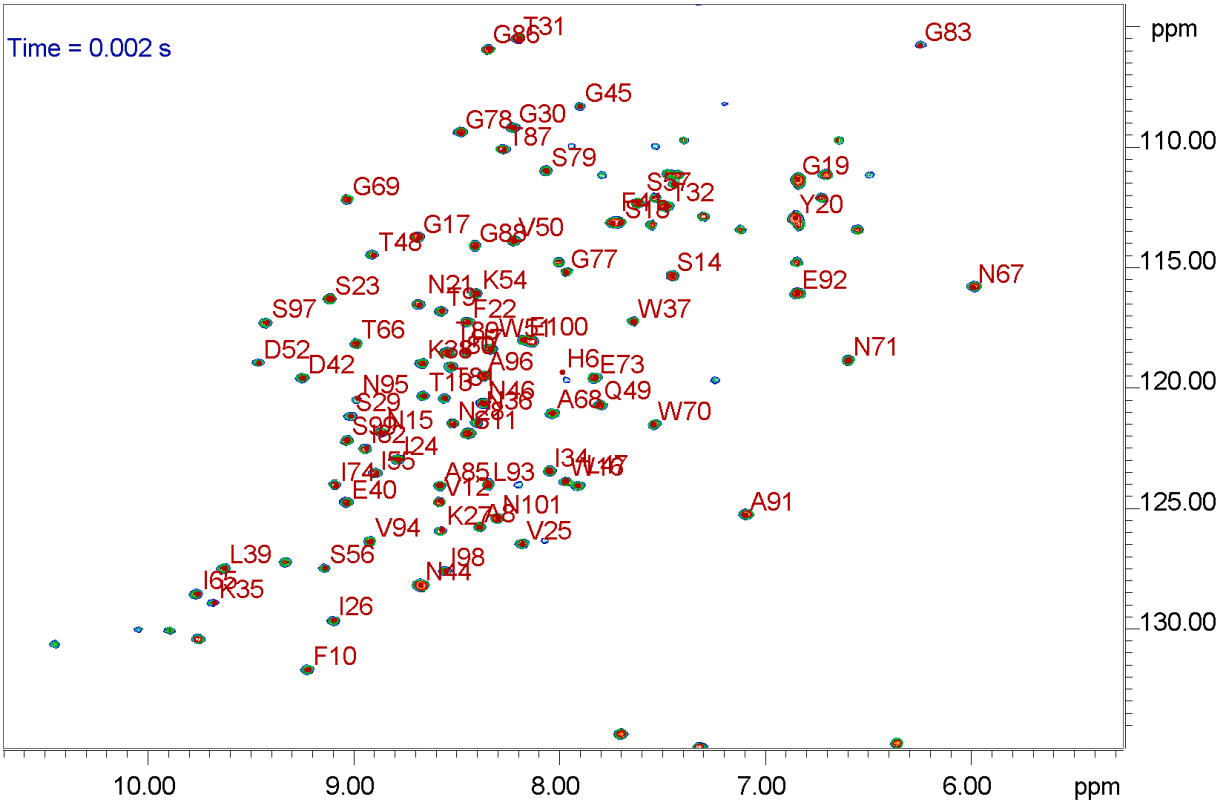
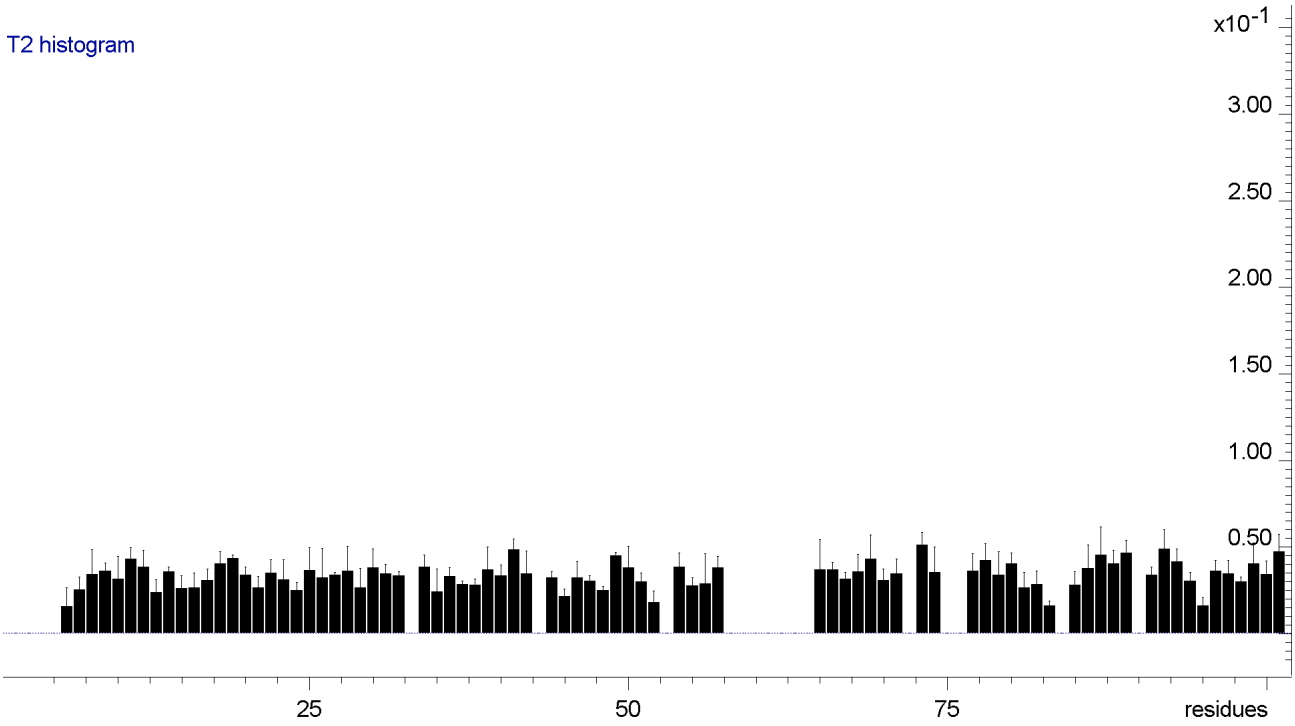
• T2 Analysis

sample name:	15N-BaCBM2 (107 uM) in 25 mM NaAc pH 5.0 10 mM NaCl, 10% D2O
Description/Title:	0.5 mM Gd
Origin:	in-house
Date of preparation:	18 Jan 2024
Solvent:	D2O
pH:	7.0
Sample tube:	normal
Tube diameter (mm):	3
Concentration (mM):	10.00
Temperature (K):	308.0
Weight (Daltons):	8900
Correlation time (ns):	4.00
Labelling:	15N
Sequence format:	FASTA file
Sequence file:	???
PDB file:	???


Time = 0.002 s
ppm
110.00
115.00
120.00
125.00
130.00
10.00
9.00
8.00
7.00
6.00
ppm
T31
G86
G83
G45
G78
G30
T87
S79
G69
G19
T32
Y20
G17
G88
V50
T48
G77
S14
E92
N67
S23
N21
K54
S97
F22
W37
T66
E100
D52
D42
A96
H6
E73
N71
N95
Q49
S29
A68
W70
N15
I24
I55
I74
A85
L93
E40
V12
N101
A91
V94
V25
L39
S56
I98
N44
K35
I26
F10


T2 histogram
x10-1
3.00
2.50
2.00
1.50
1.00
0.50
25
50
75
residues

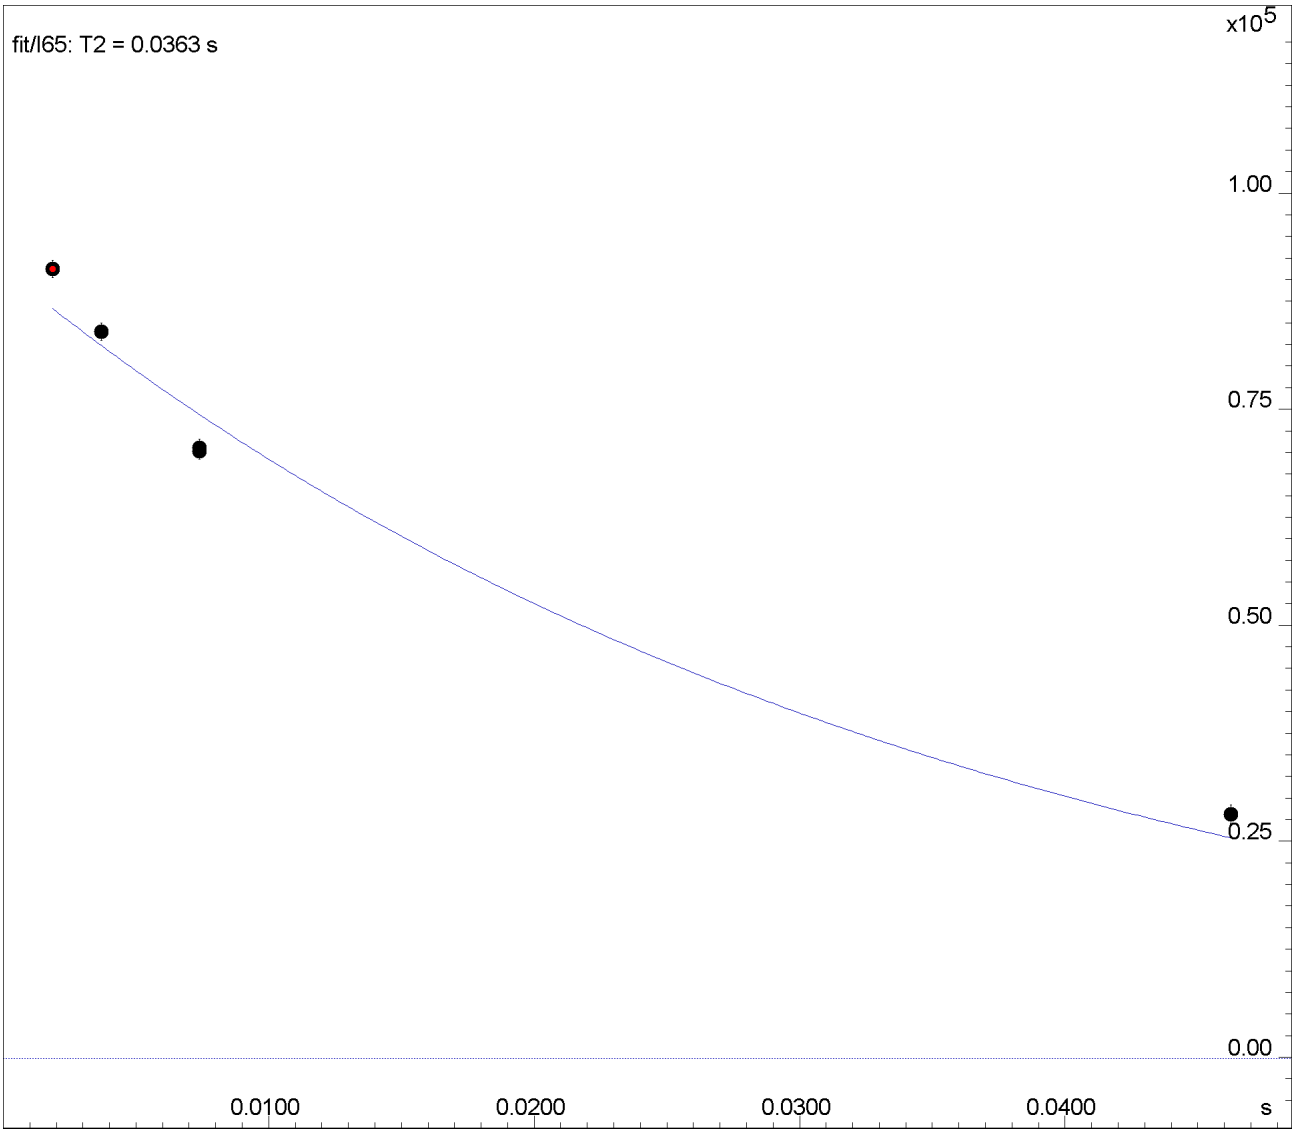
Fitted function:	f(t) = Io * exp (-t/T)
Random error estimation of data:	RMS per spectrum (or trace/plane)
Systematic error estimation of data:	worst case per peak scenario
Fit parameter Error estimation method:	from fit using arbitrary y uncertainties
Confidence level:	95%
Used peaks:	peaks from C:\Users\susanntr\OneDrive - NTNU\NMR_data\BaCBM2\50\pdata\1\peaklist.xml
Used integrals:	peak intensities
Used Time:	all values (including replicates) used

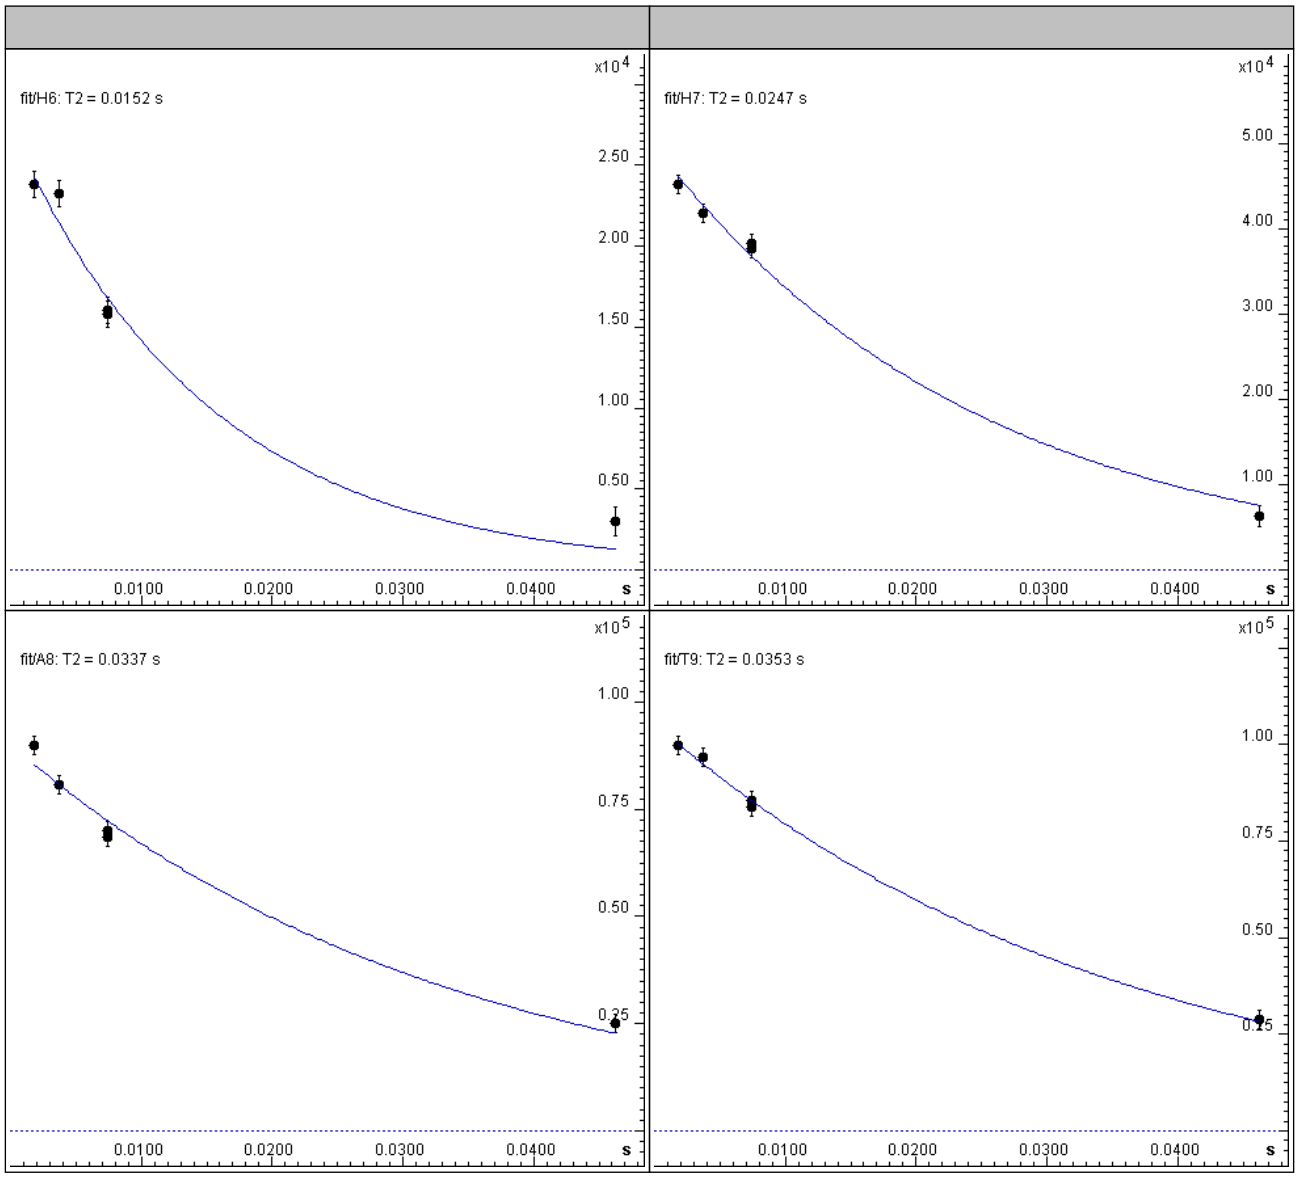
Peak name	F1 [ppm]	F2 [ppm]	Io	error	T2 [s]	error	fitInfo
H6	119.318	7.984	2.74e+04	6667	0.0152	0.01095	Done
H7	118.470	8.447	4.97e+04	4079	0.0247	0.007427	Done
A8	125.738	8.383	9.03e+04	9563	0.0337	0.01411	Done
T9	116.775	8.565	1.06e+05	3685	0.0353	0.004914	Done
F10	131.674	9.216	9.64e+04	1.056e+04	0.0308	0.01304	Done
S11	121.862	8.436	1.43e+05	5360	0.0422	0.006651	Done
V12	124.648	8.577	1.17e+05	7467	0.0376	0.009772	Done
T13	120.287	8.653	9.37e+04	8378	0.0232	0.007457	Done
S14	115.321	7.450	1.71e+05	3675	0.0352	0.003019	Done
N15	121.862	8.858	1.04e+05	8183	0.0256	0.007457	Done
W16	123.800	7.966	9.63e+04	8735	0.0259	0.008716	Done
G17	113.746	8.682	1.27e+05	7137	0.0301	0.006515	Done
S18	113.141	7.702	1.52e+05	6691	0.0397	0.007195	Done
G19	111.324	6.839	2.17e+05	2586	0.0425	0.002131	Done
Y20	112.898	6.851	2.23e+05	7743	0.0333	0.004559	Done
N21	116.532	8.676	9.56e+04	6736	0.0258	0.006756	Done
F22	117.259	8.442	1.04e+05	5907	0.0343	0.007759	Done
S23	116.290	9.111	1.15e+05	1.113e+04	0.0306	0.01140	Done
I24	122.952	8.776	1.05e+05	5489	0.0246	0.004711	Done
V25	126.465	8.177	1.11e+05	1.001e+04	0.0357	0.01291	Done
I26	129.614	9.093	8.50e+04	1.167e+04	0.0318	0.01704	Done
K27	125.859	8.565	8.81e+04	1244	0.0330	0.001833	Done
N28	121.499	8.512	8.76e+04	8875	0.0355	0.01439	Done
S29	121.135	9.011	6.26e+04	7153	0.0261	0.01107	Done
G30	109.143	8.219	1.18e+05	8479	0.0373	0.01089	Done
T31	105.509	8.195	9.97e+04	4058	0.0340	0.005472	Done
T32	112.414	7.479	1.51e+05	2708	0.0328	0.002320	Done
I34	123.437	8.043	1.03e+05	4766	0.0376	0.007080	Done
K35	128.888	9.674	5.15e+04	7906	0.0238	0.01323	Done
N36	121.377	8.395	8.74e+04	3495	0.0322	0.005042	Done
W37	117.259	7.638	9.61e+04	1965	0.0280	0.002161	Done
K38	118.955	8.659	9.28e+04	3242	0.0274	0.003605	Done
L39	127.434	9.621	8.65e+04	7736	0.0361	0.01300	Done
E40	124.769	9.028	1.07e+05	5062	0.0330	0.006152	Done

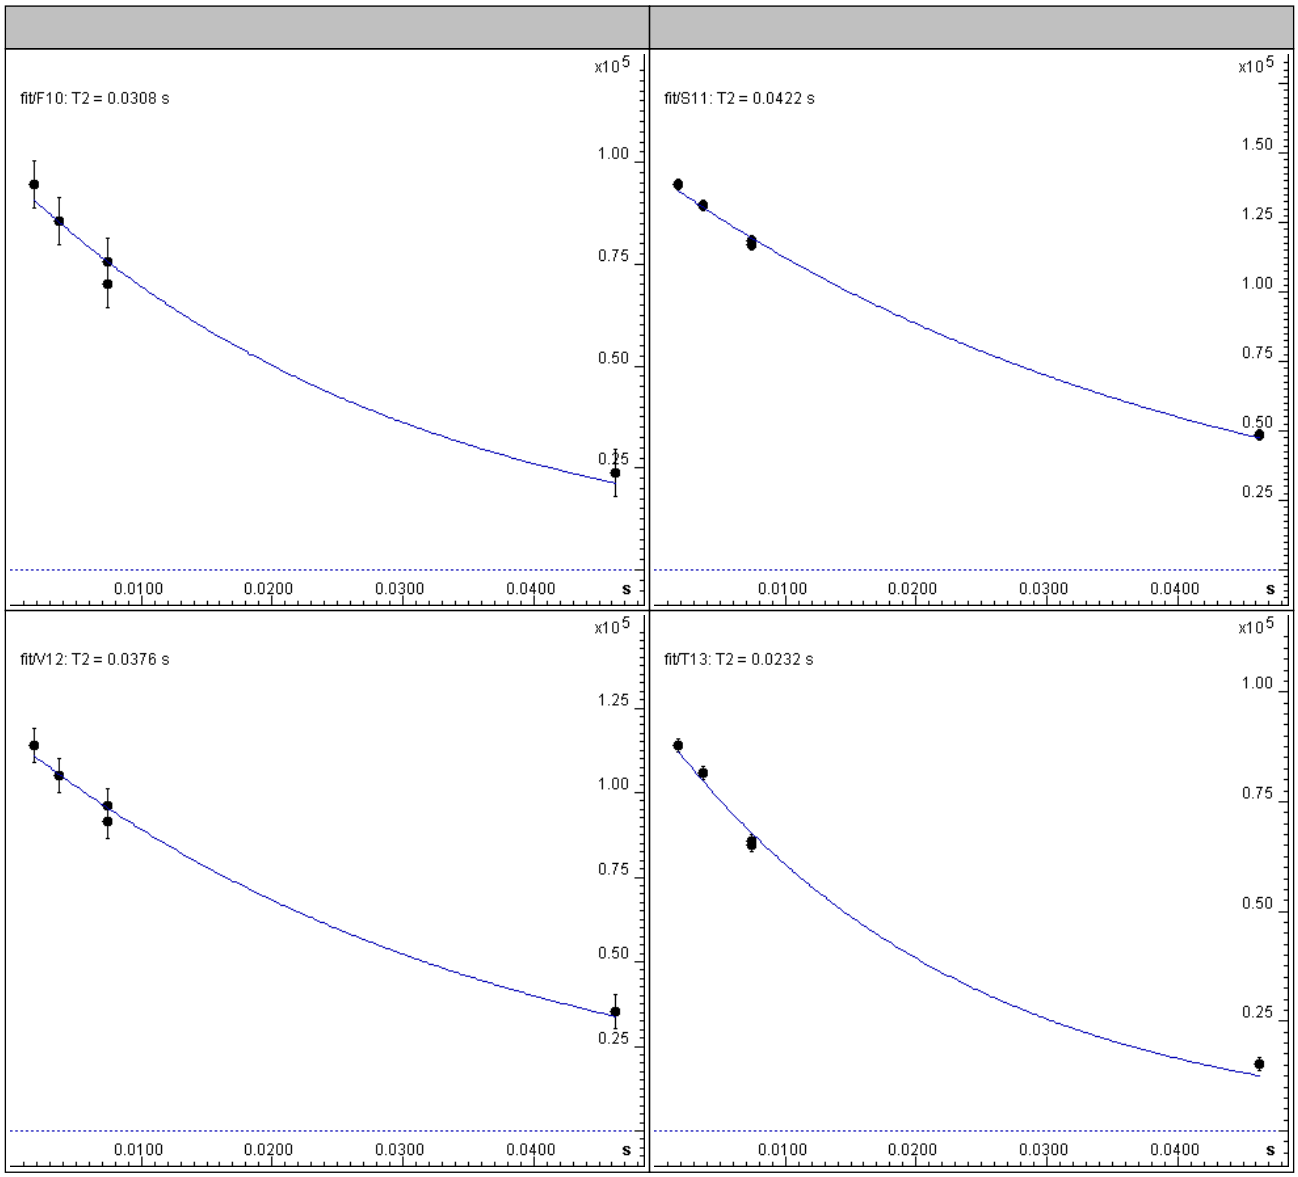
Peak name	F1 [ppm]	F2 [ppm]	Io	error	T2 [s]	error	fitInfo
F41	113.141	7.737	1.71e+05	5058	0.0476	0.006153	Done
D42	119.561	9.240	1.05e+05	1.027e+04	0.0338	0.01309	Done
N44	128.161	8.670	2.13e+05	6021	0.0316	0.003470	Done
G45	108.295	7.896	6.84e+04	3953	0.0212	0.004281	Done
N46	120.651	8.365	8.98e+04	6854	0.0316	0.009394	Done
L47	124.042	7.908	9.73e+04	2784	0.0296	0.003249	Done
T48	114.473	8.899	9.34e+04	2511	0.0246	0.002421	Done
Q49	120.651	7.802	1.52e+05	1576	0.0440	0.001940	Done
V50	113.867	8.219	1.26e+05	1.042e+04	0.0374	0.01251	Done
W51	118.349	8.330	1.00e+05	4470	0.0293	0.005007	Done
D52	118.955	9.457	6.34e+04	7278	0.0176	0.006499	Done
K54	116.048	8.395	1.12e+05	5929	0.0377	0.008122	Done
I55	123.558	8.888	1.01e+05	4549	0.0272	0.004570	Done
S56	127.434	9.134	7.57e+04	1.231e+04	0.0281	0.01730	Done
S57	112.293	7.614	1.42e+05	6332	0.0375	0.006767	Done
I65	128.524	9.750	9.28e+04	1.093e+04	0.0363	0.01722	Done
T66	118.107	8.981	1.08e+05	3200	0.0363	0.004343	Done
N67	115.805	5.989	1.33e+05	4265	0.0309	0.003840	Done
A68	121.014	8.031	1.08e+05	7928	0.0350	0.01022	Done
G69	112.172	9.023	1.15e+05	8949	0.0424	0.01391	Done
W70	121.499	7.538	1.23e+05	6946	0.0301	0.006526	Done
N71	118.834	6.593	1.06e+05	6587	0.0340	0.008377	Done
E73	119.561	7.825	1.25e+05	4010	0.0504	0.007206	Done
I74	124.042	9.081	8.74e+04	9274	0.0346	0.01459	Done
G77	115.200	7.966	9.62e+04	6851	0.0353	0.01004	Done
G78	109.386	8.477	1.24e+05	6994	0.0415	0.009824	Done
S79	110.960	8.060	1.03e+05	1.056e+04	0.0333	0.01337	Done
I80	119.076	8.518	1.13e+05	4420	0.0398	0.006444	Done
T81	120.408	8.553	7.65e+04	7006	0.0259	0.008811	Done
I82	122.468	8.935	9.78e+04	7073	0.0280	0.007640	Done
G83	105.752	6.247	6.04e+04	3643	0.0158	0.002870	Done
A85	124.042	8.577	1.05e+05	7673	0.0276	0.007630	Done
G86	105.873	8.342	1.10e+05	9827	0.0371	0.01344	Done
T87	110.112	8.266	9.89e+04	8436	0.0444	0.01617	Done
G88	114.110	8.406	1.07e+05	4982	0.0398	0.007664	Done
T89	118.470	8.541	1.54e+05	5663	0.0457	0.007244	Done
A91	125.254	7.092	1.41e+05	5077	0.0333	0.004721	Done
E92	116.048	6.839	1.65e+05	8752	0.0481	0.01123	Done
L93	124.042	8.342	1.13e+05	4934	0.0409	0.007434	Done
V94	126.344	8.911	1.05e+05	4567	0.0297	0.004940	Done
N95	120.408	8.976	4.71e+04	4533	0.0159	0.004637	Done
A96	119.439	8.365	1.59e+05	6823	0.0355	0.006104	Done
S97	117.259	9.416	1.07e+05	6270	0.0340	0.007920	Done
I98	127.555	8.547	7.20e+04	1879	0.0295	0.002944	Done
S99	122.104	9.028	9.95e+04	7185	0.0396	0.01177	Done

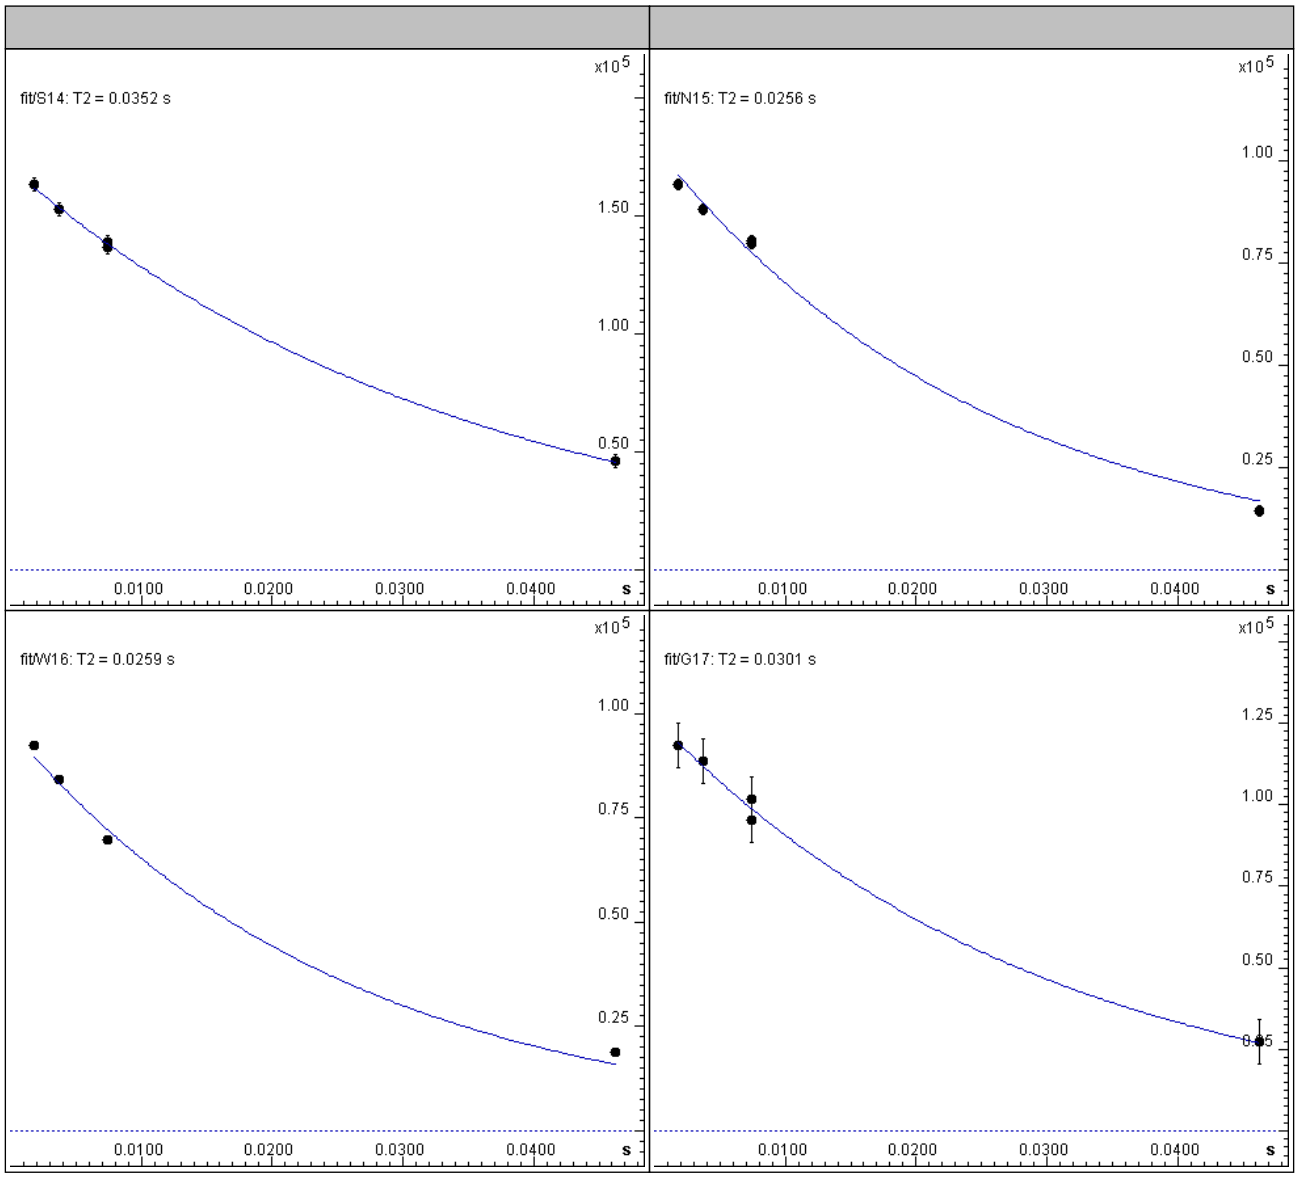
Peak name	F1 [ppm]	F2 [ppm]	Io	error	T2 [s]	error	fitInfo
E100	117.986	8.166	1.09e+05	6348	0.0334	0.007680	Done
N101	125.375	8.295	1.47e+05	7232	0.0464	0.009861	Done

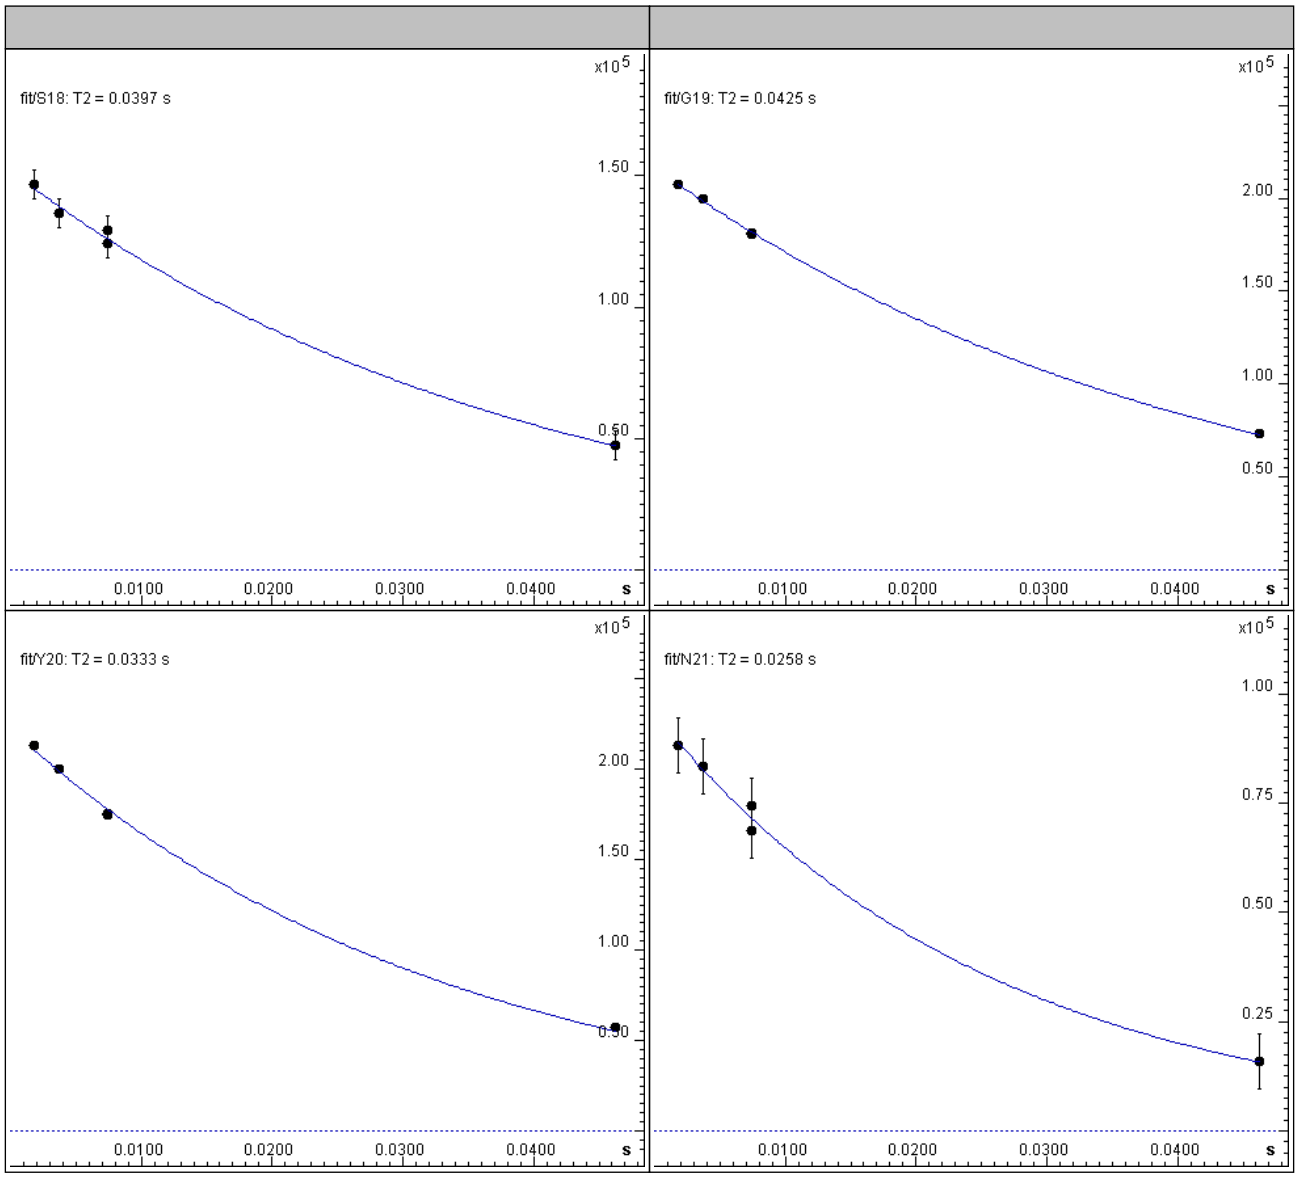
Current fit display

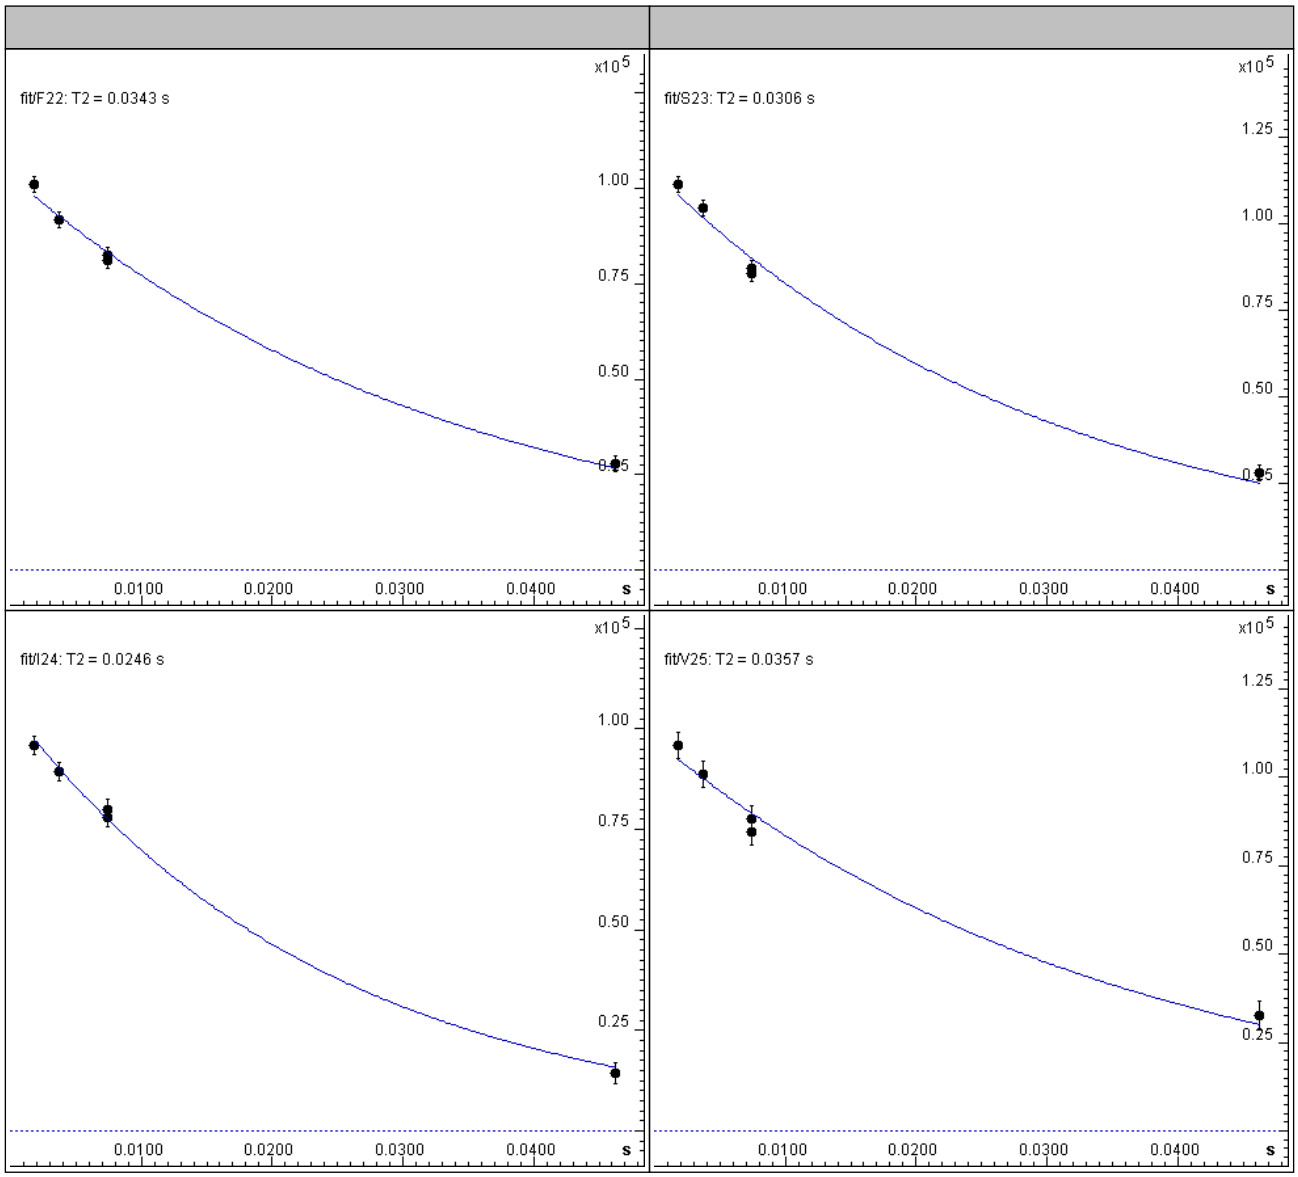


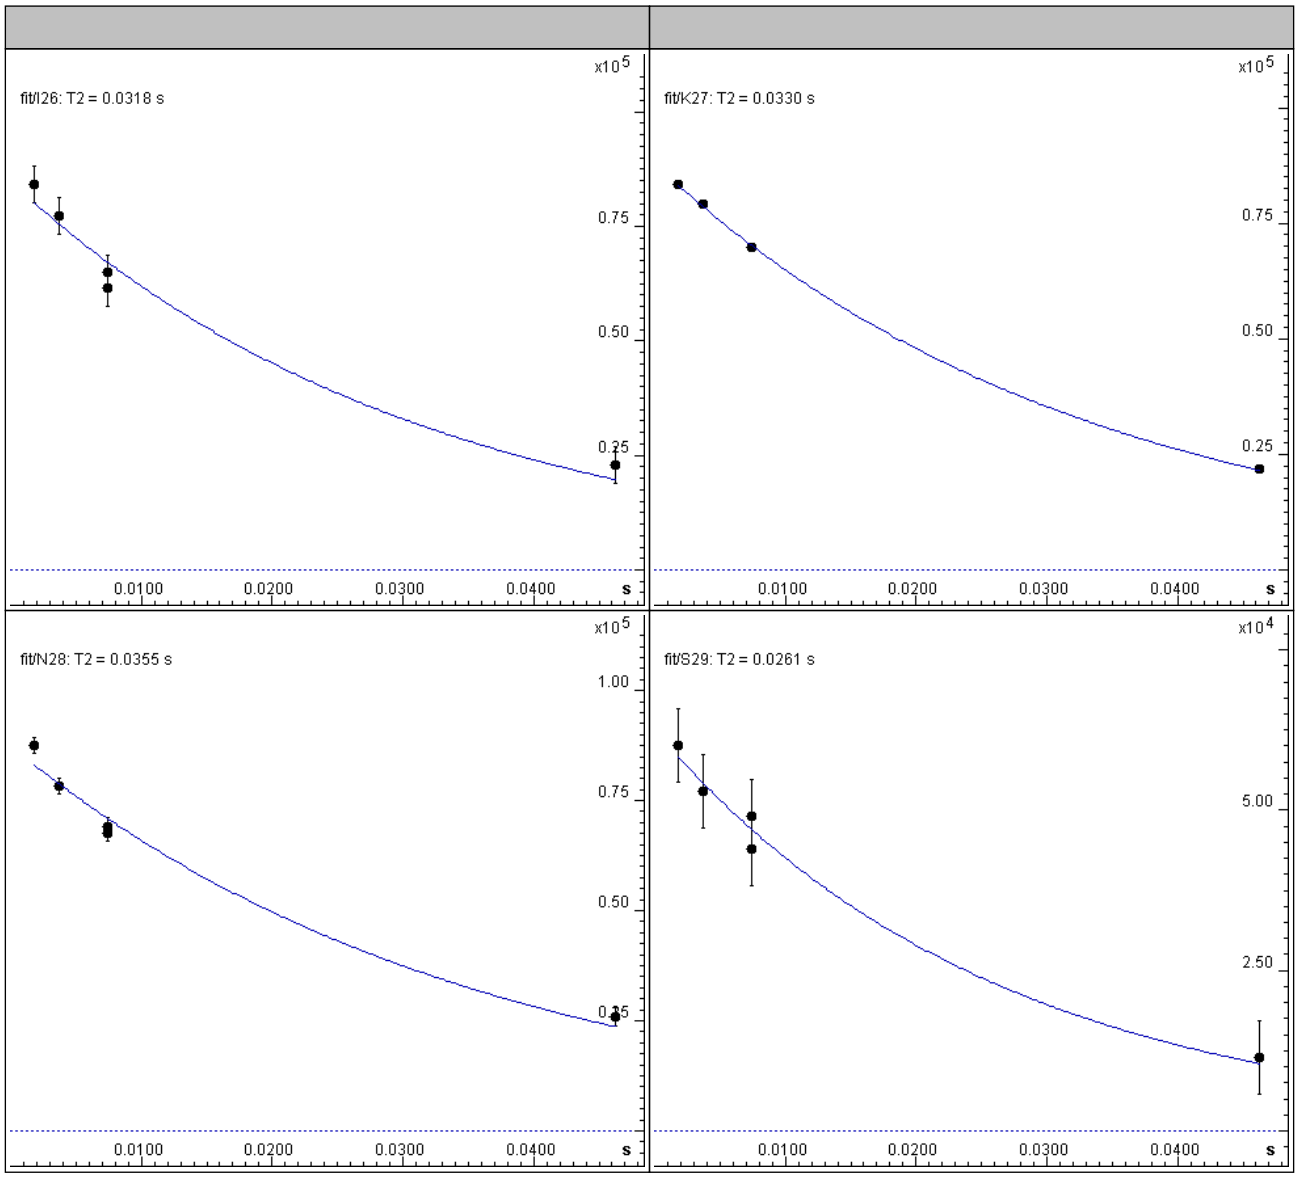

fit/H6: T2 = 0.0152 s
x10 4
2.50
2.00
1.50
1.00
0.50
0.0100
0.0200
0.0300
0.0400
s
fit/H7: T2 = 0.0247 s
x10 4
5.00
4.00
3.00
2.00
1.00
0.0100
0.0200
0.0300
0.0400
s
fit/A8: T2 = 0.0337 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/T9: T2 = 0.0353 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s

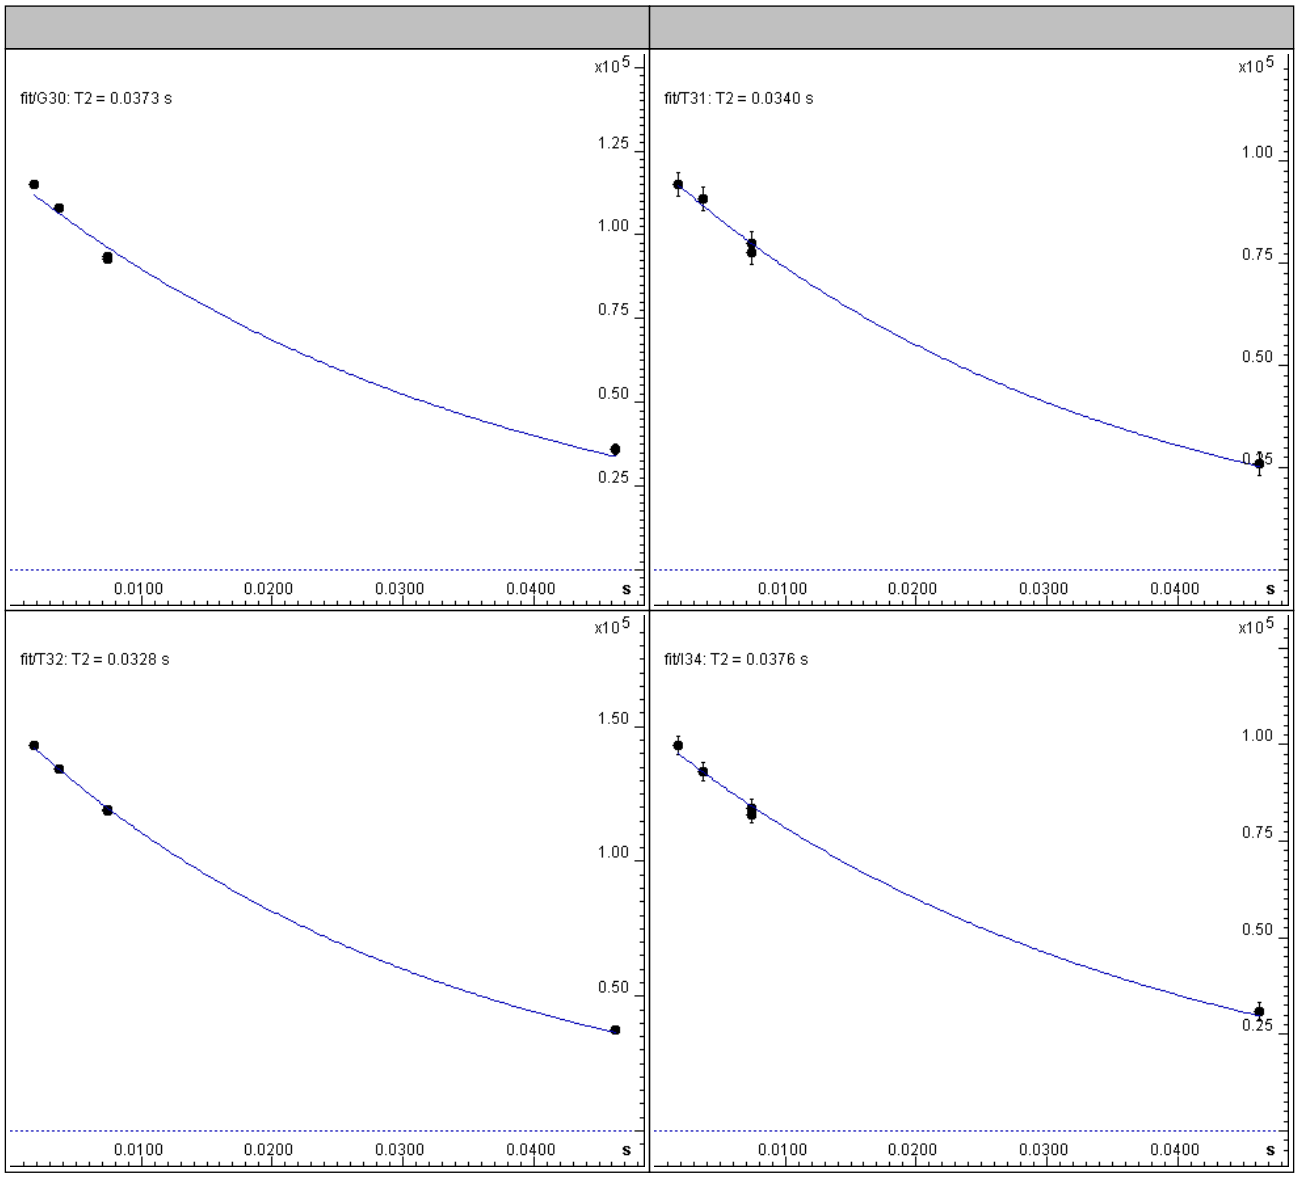

fit/F10: T2 = 0.0308 s
fit/S11: T2 = 0.0422 s
fit/V12: T2 = 0.0376 s
fit/T13: T2 = 0.0232 s
x10^5
0.0100
0.0200
0.0300
0.0400
s

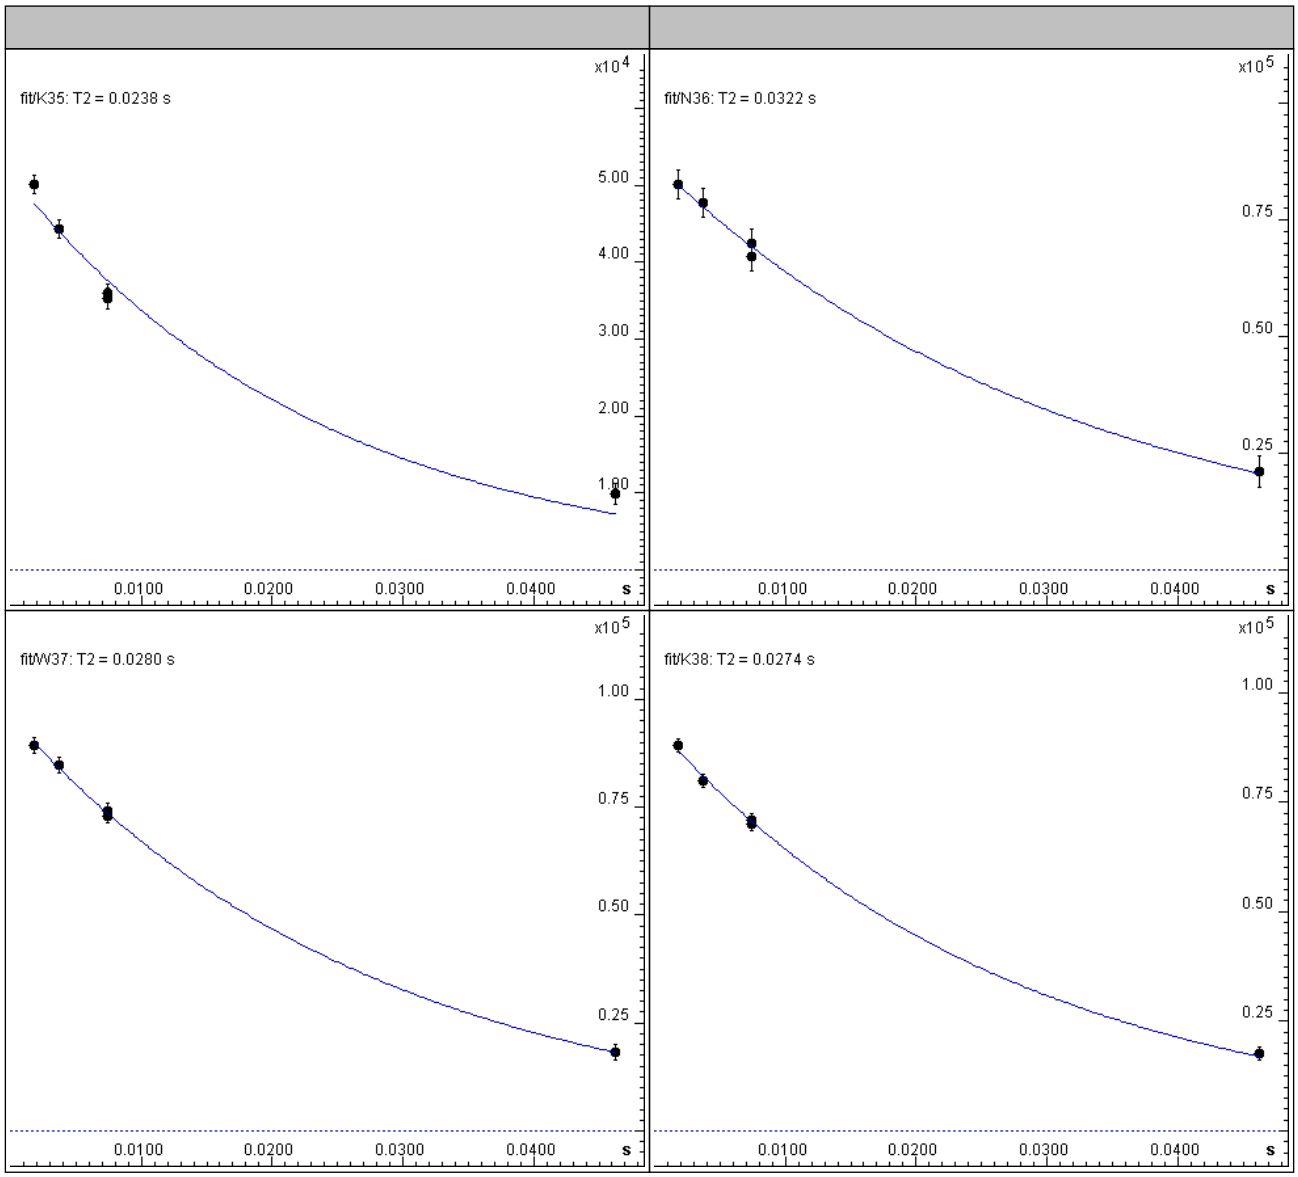

fit/S14: T2 = 0.0352 s
fit/N15: T2 = 0.0256 s
fit/W16: T2 = 0.0259 s
fit/G17: T2 = 0.0301 s
x10 5
0.0100
0.0200
0.0300
0.0400
s

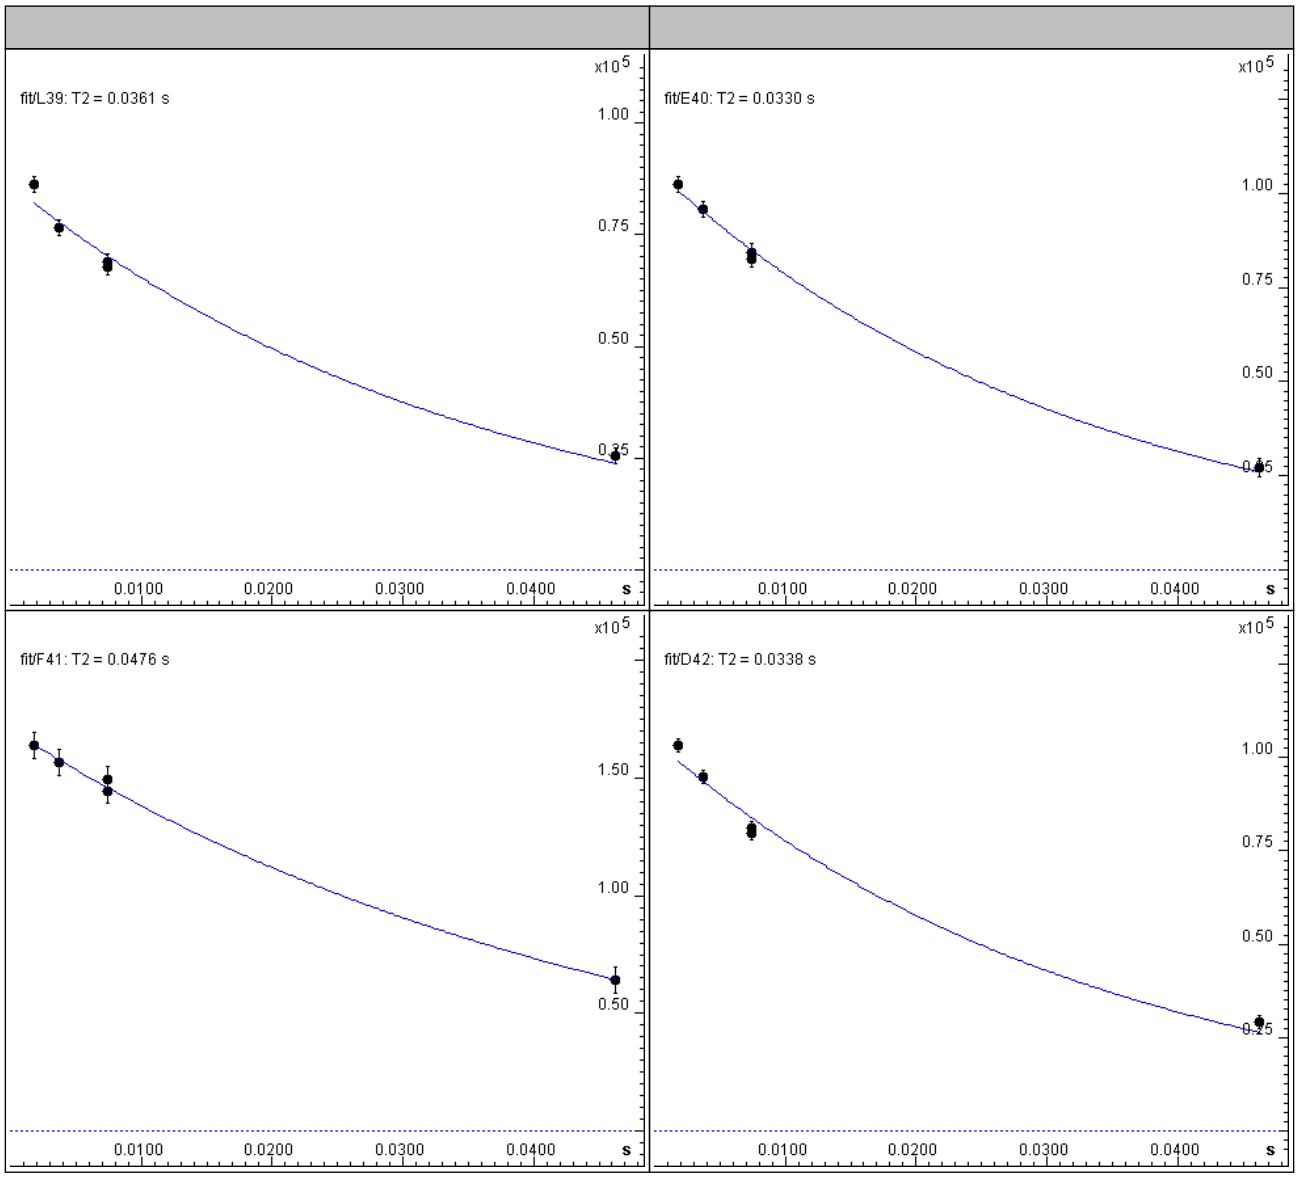

fit/S18: T2 = 0.0397 s
fit/G19: T2 = 0.0425 s
fit/Y20: T2 = 0.0333 s
fit/N21: T2 = 0.0258 s
x10 5
0.0100
0.0200
0.0300
0.0400
s

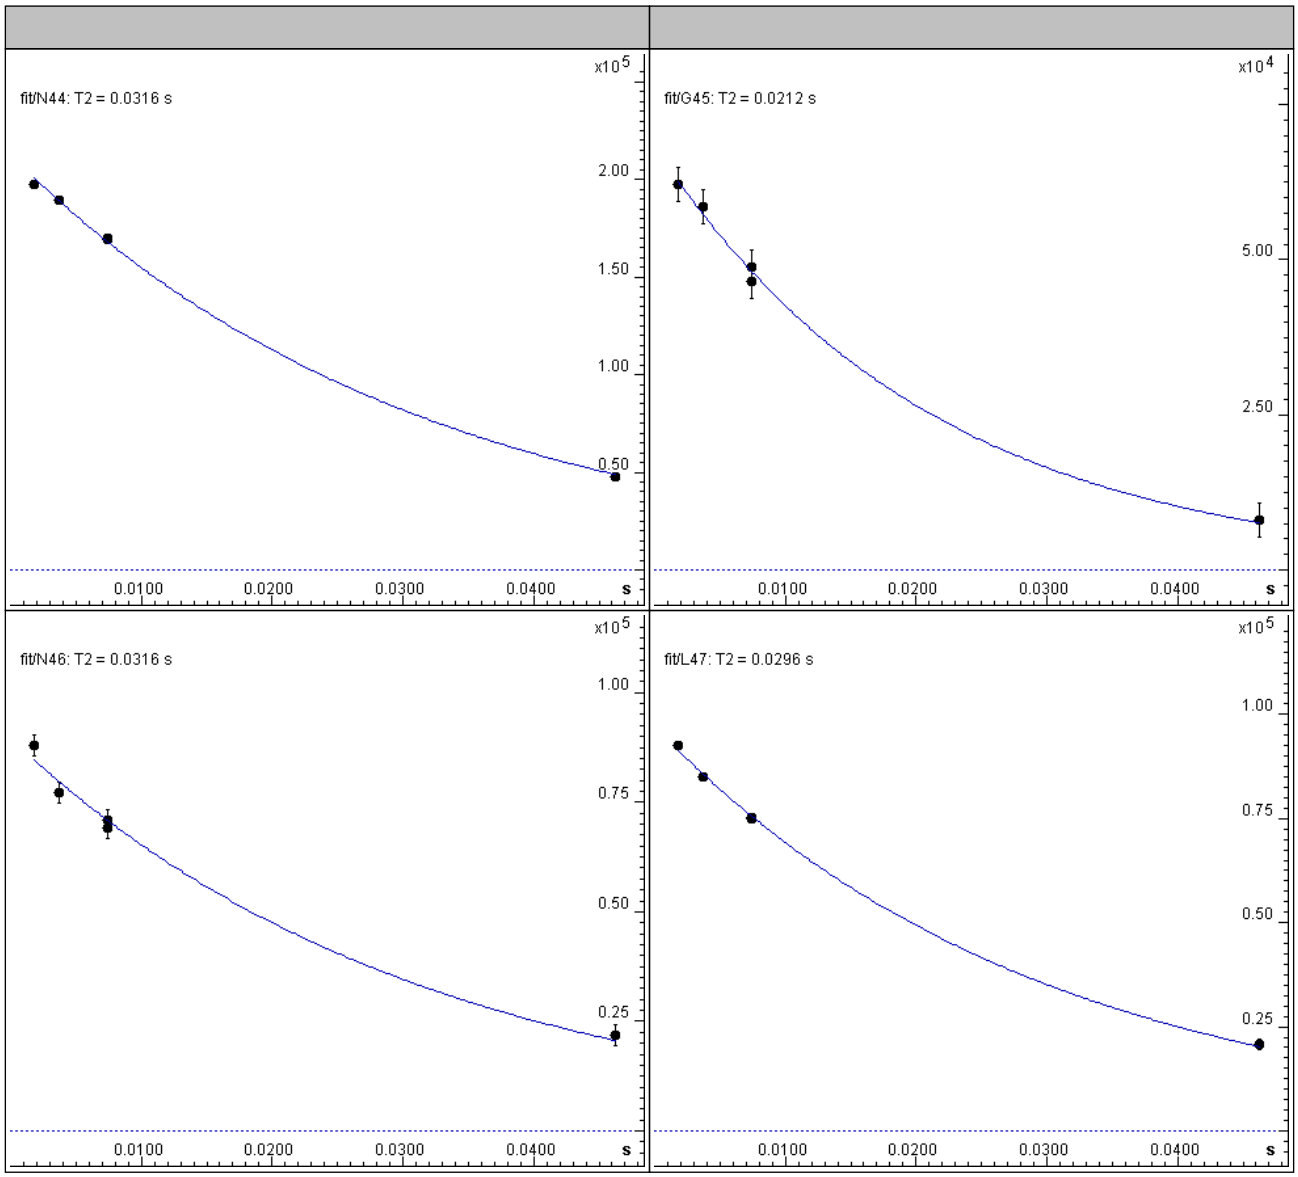

fit/F22: T2 = 0.0343 s
fit/S23: T2 = 0.0306 s
fit/I24: T2 = 0.0246 s
fit/V25: T2 = 0.0357 s
x10 5
1.25
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s

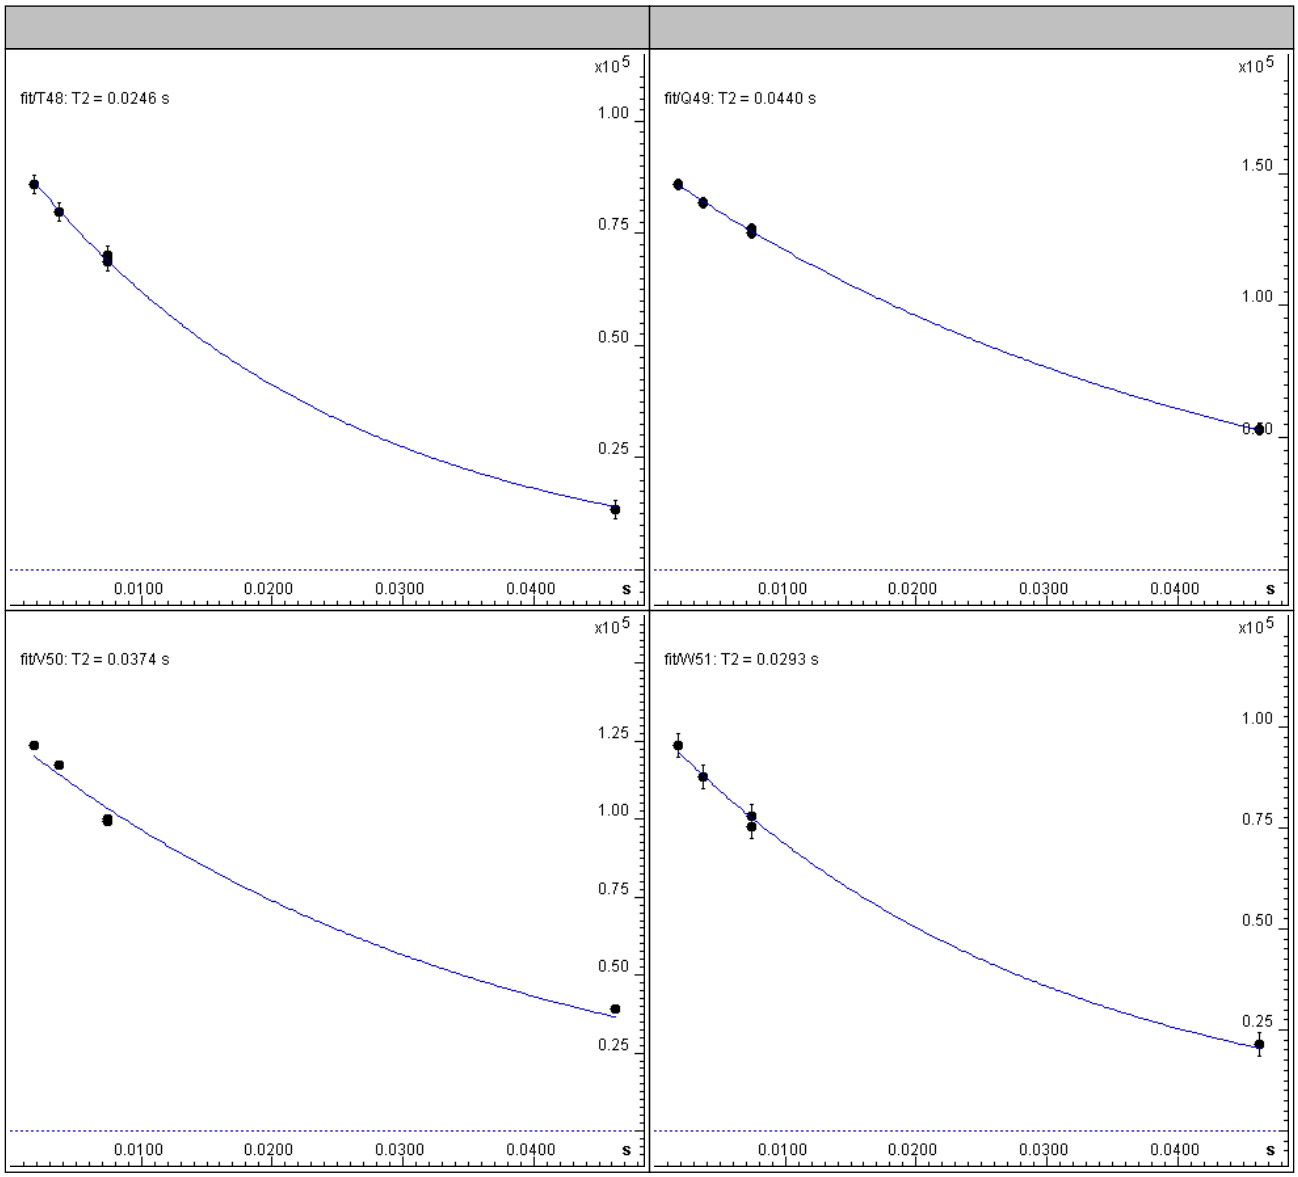

fit/I26: T2 = 0.0318 s
x10 5
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/K27: T2 = 0.0330 s
x10 5
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/N28: T2 = 0.0355 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/S29: T2 = 0.0261 s
x10 4
5.00
2.50
0.0100
0.0200
0.0300
0.0400
s

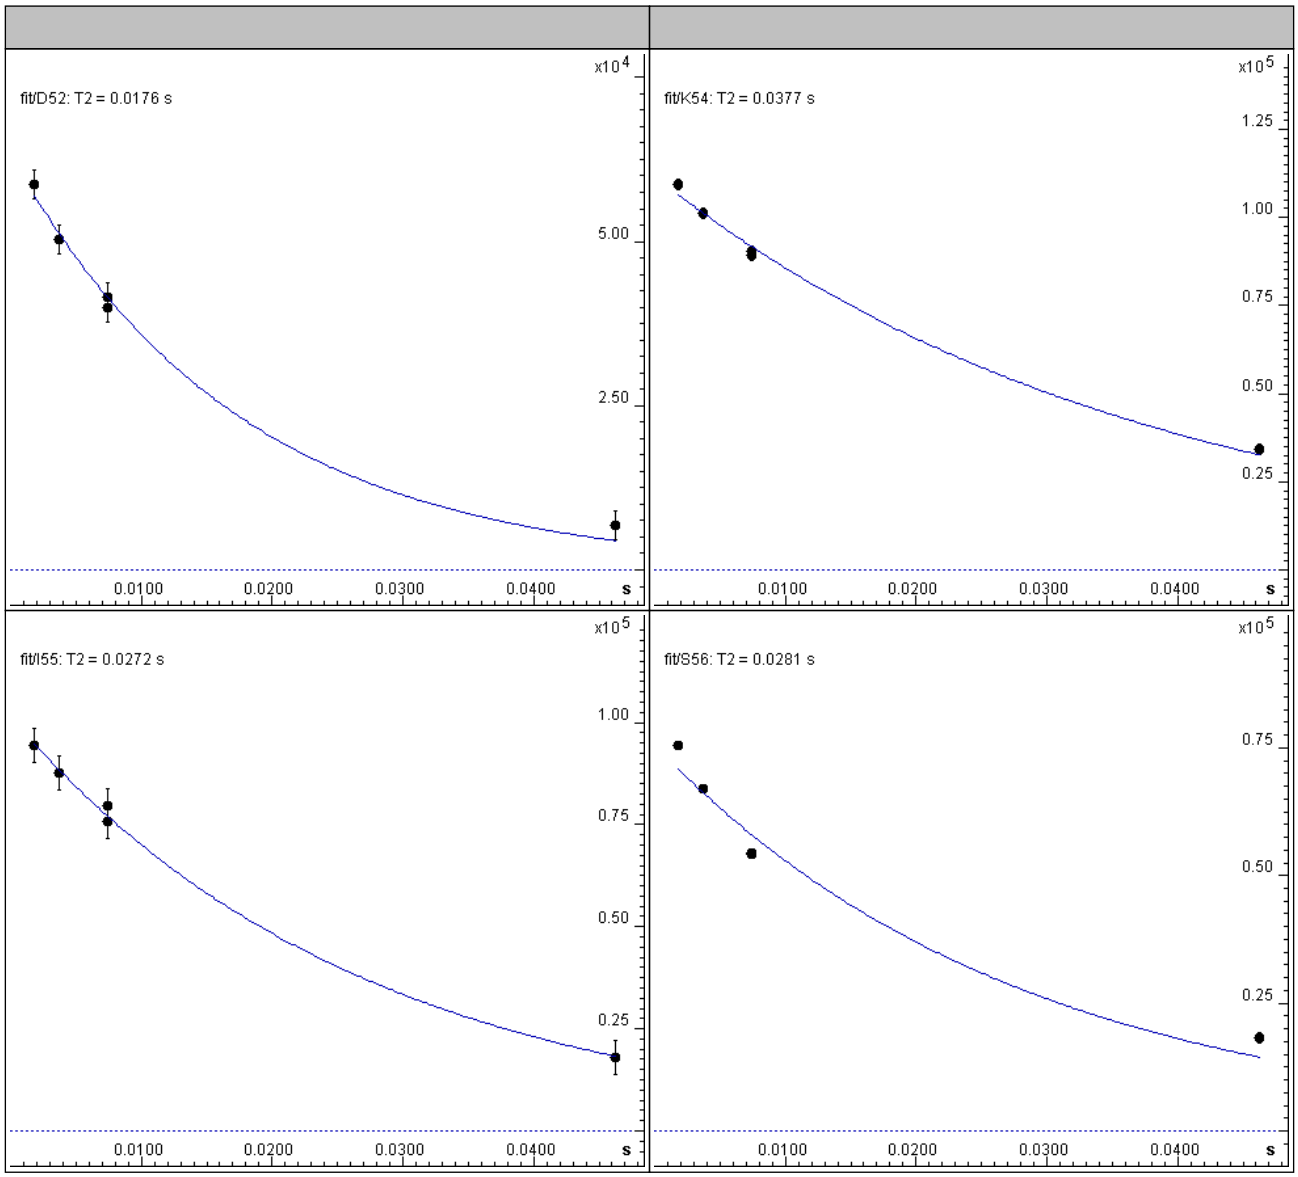

fit/G30: T2 = 0.0373 s
fit/T31: T2 = 0.0340 s
fit/T32: T2 = 0.0328 s
fit/I34: T2 = 0.0376 s
x10^5
0.0100
0.0200
0.0300
0.0400
s

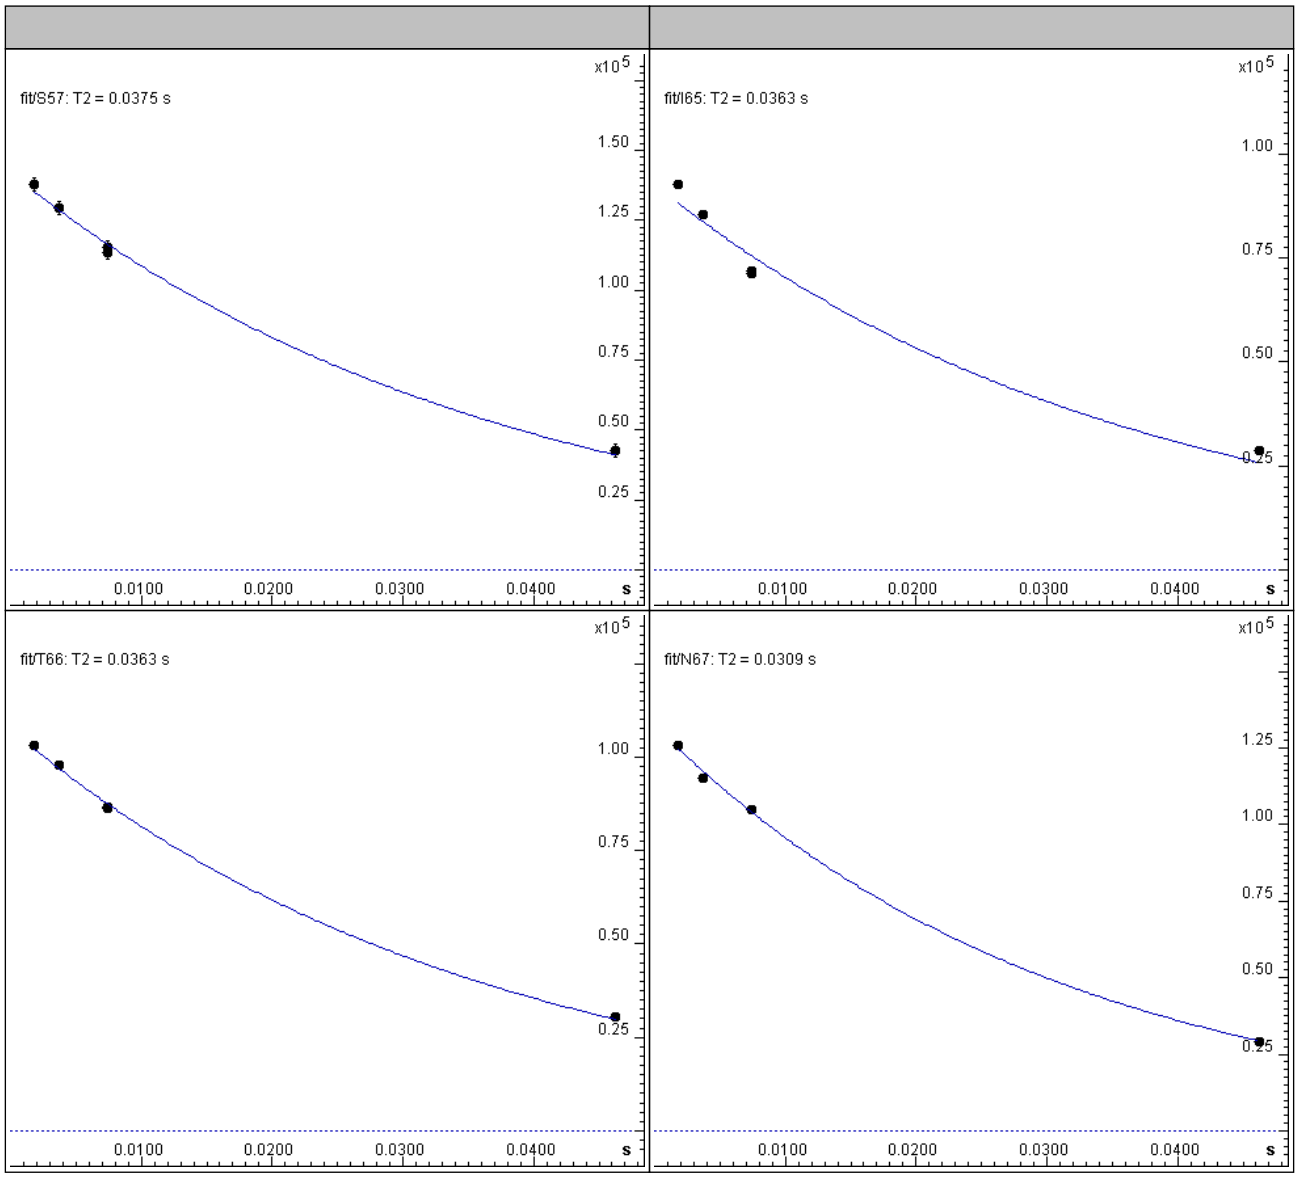

fit/K35: T2 = 0.0238 s
x10 4
5.00
4.00
3.00
2.00
1.80
0.0100
0.0200
0.0300
0.0400
s
fit/N36: T2 = 0.0322 s
x10 5
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/W37: T2 = 0.0280 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/K38: T2 = 0.0274 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s

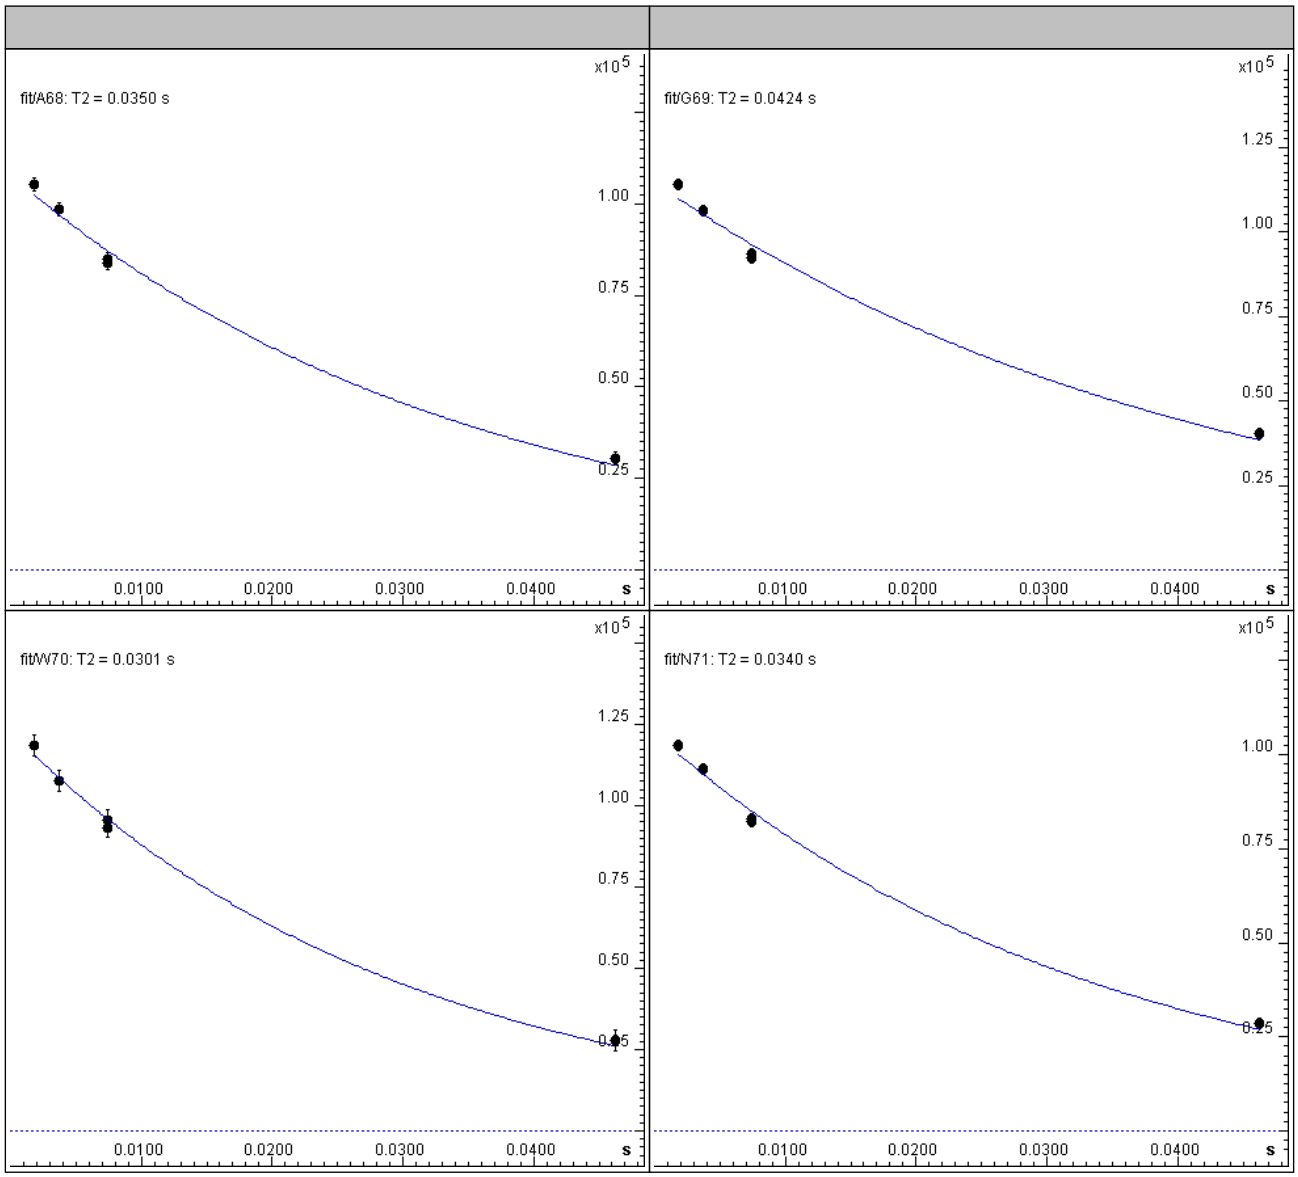

fit/L39: T2 = 0.0361 s
fit/E40: T2 = 0.0330 s
fit/F41: T2 = 0.0476 s
fit/D42: T2 = 0.0338 s
x10 5
1.00
0.75
0.50
1.50
0.0100
0.0200
0.0300
0.0400
s

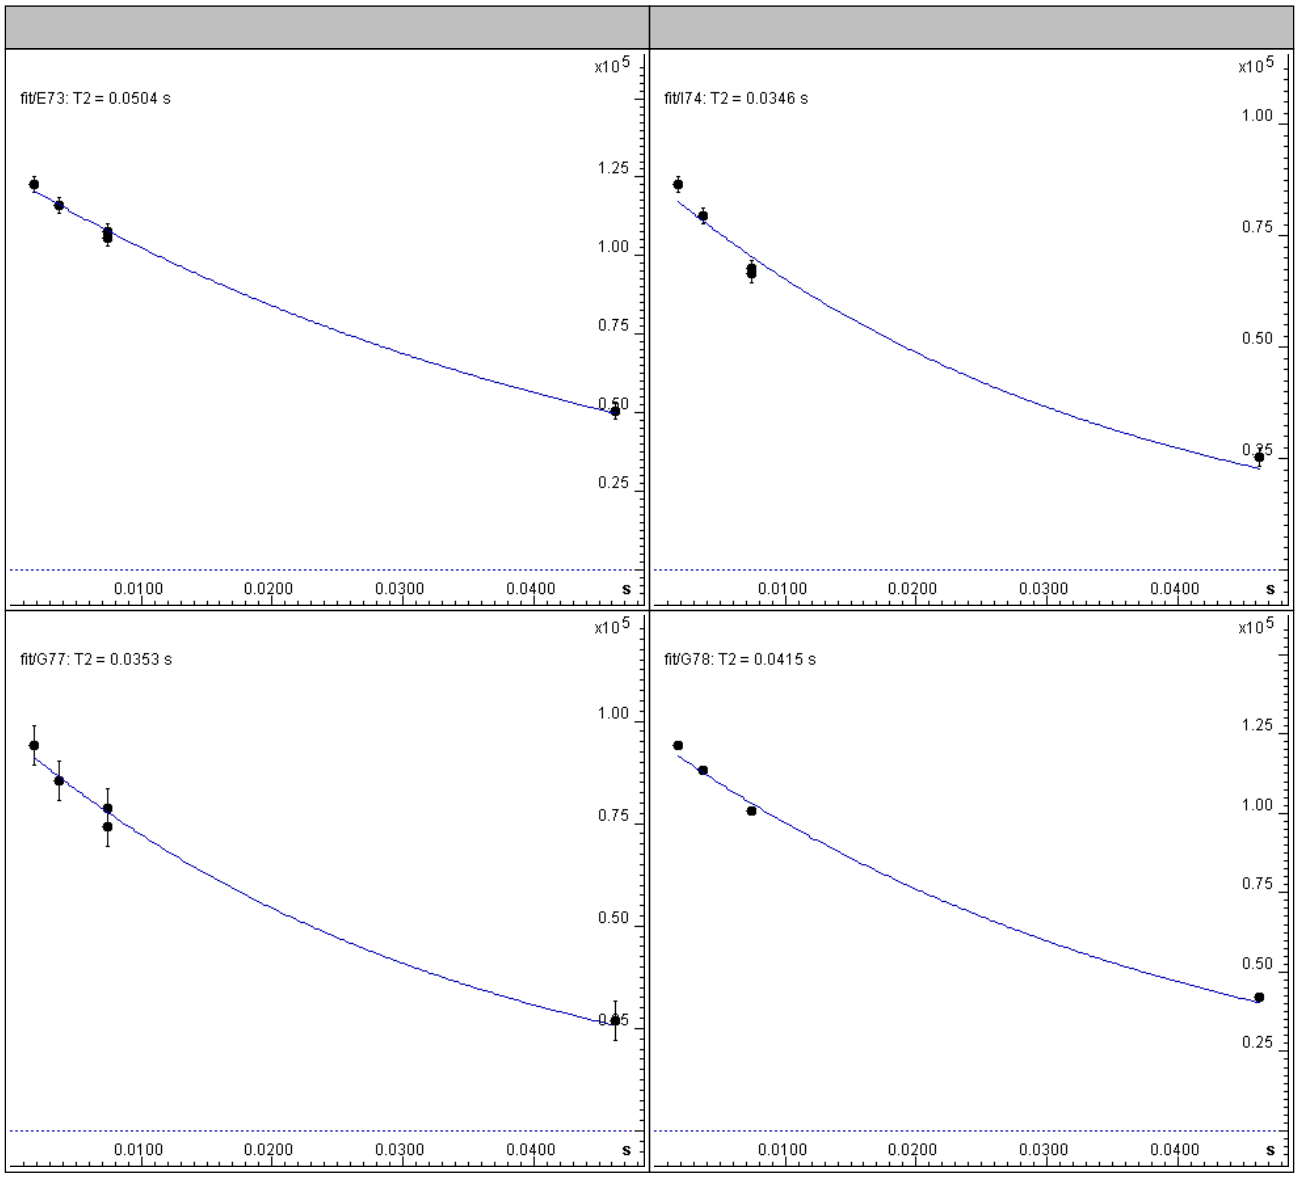

fit/N44: T2 = 0.0316 s
x10 5
2.00
1.50
1.00
0.50
0.0100
0.0200
0.0300
0.0400
s
fit/G45: T2 = 0.0212 s
x10 4
5.00
2.50
fit/N46: T2 = 0.0316 s
x10 5
1.00
0.75
0.50
0.25
fit/L47: T2 = 0.0296 s

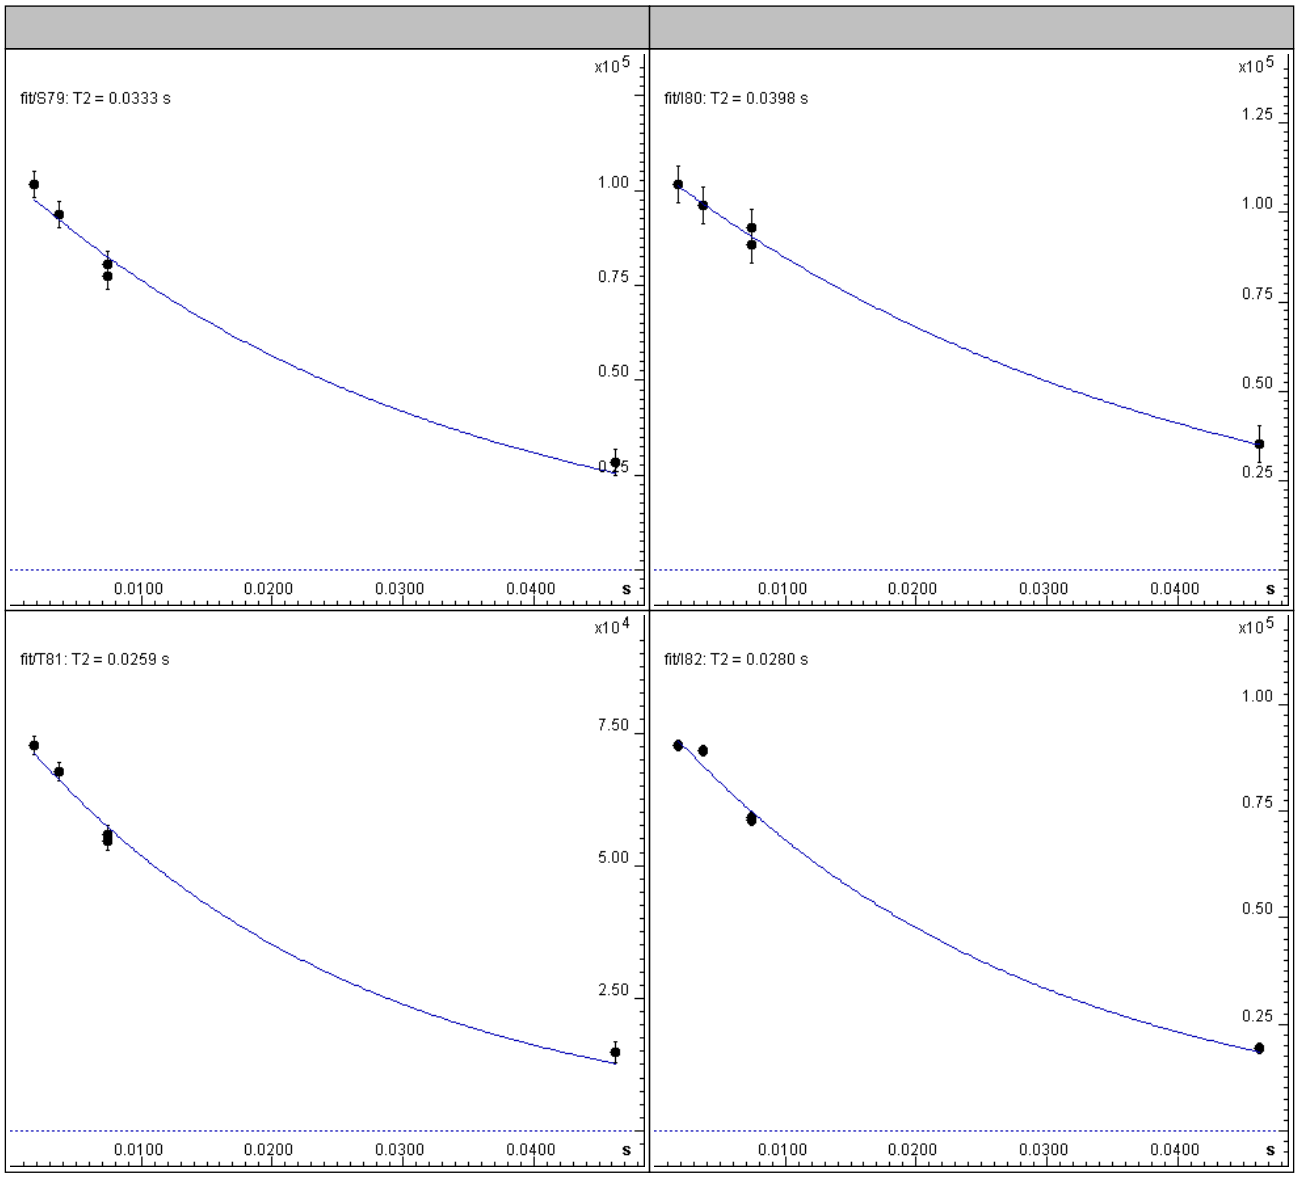

fit/T48: T2 = 0.0246 s
fit/Q49: T2 = 0.0440 s
fit/V50: T2 = 0.0374 s
fit/W51: T2 = 0.0293 s
x10^5
0.0100
0.0200
0.0300
0.0400
s

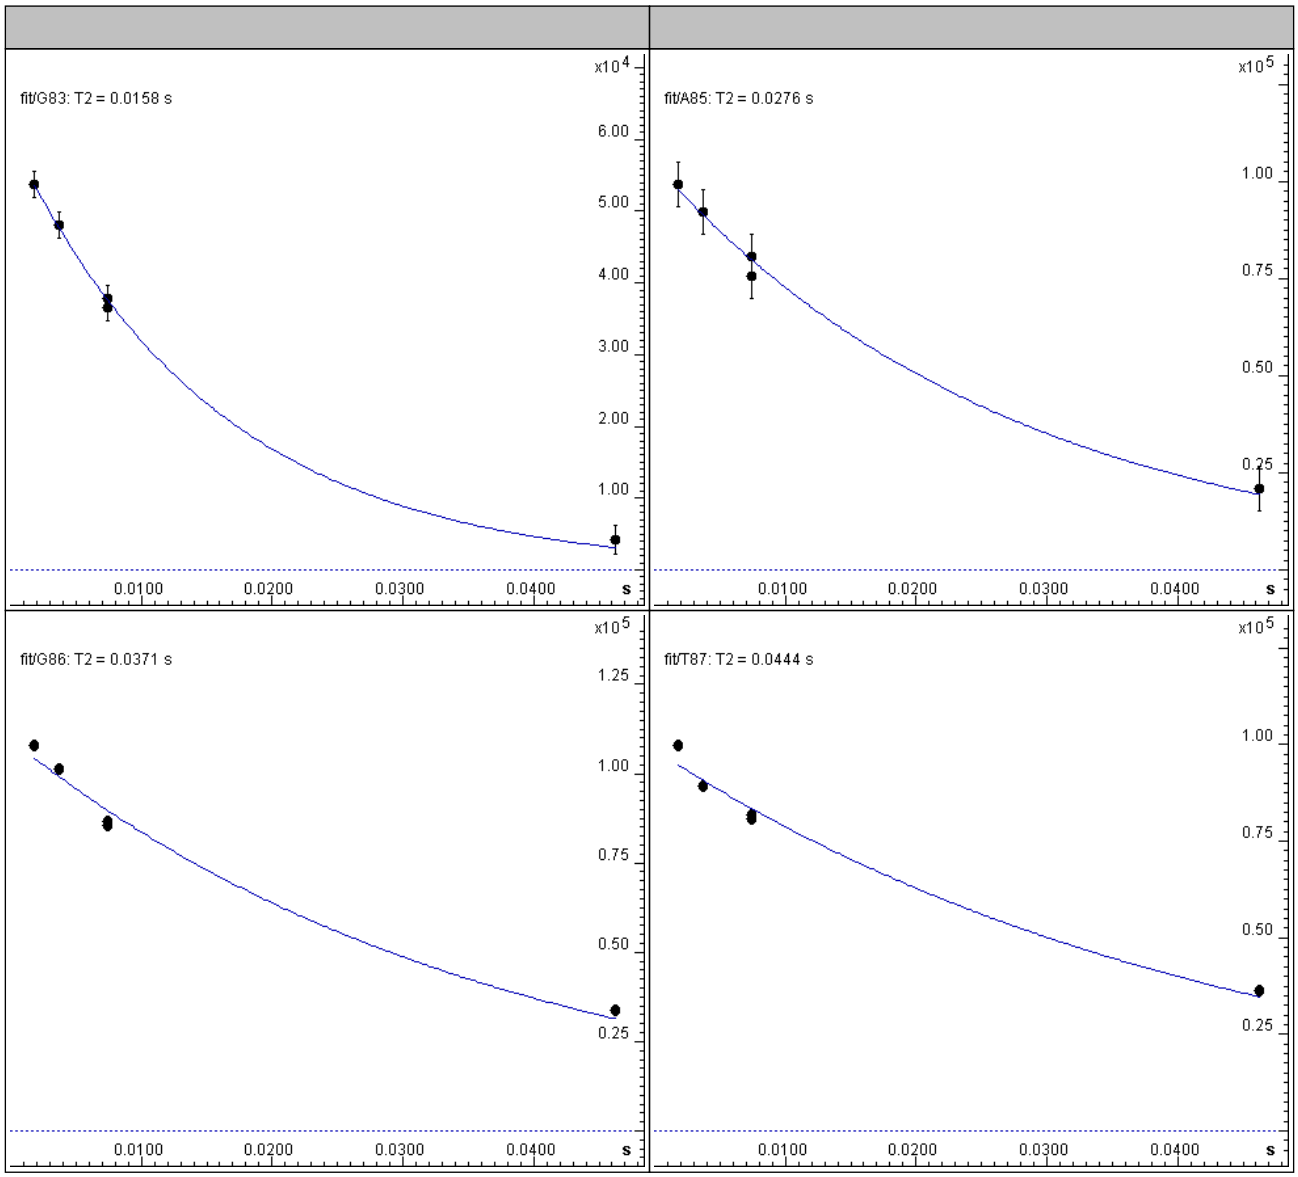

fit/D52: T2 = 0.0176 s
x10 4
5.00
2.50
0.0100
0.0200
0.0300
0.0400
s
fit/K54: T2 = 0.0377 s
x10 5
1.25
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/I55: T2 = 0.0272 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/S56: T2 = 0.0281 s
x10 5
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s

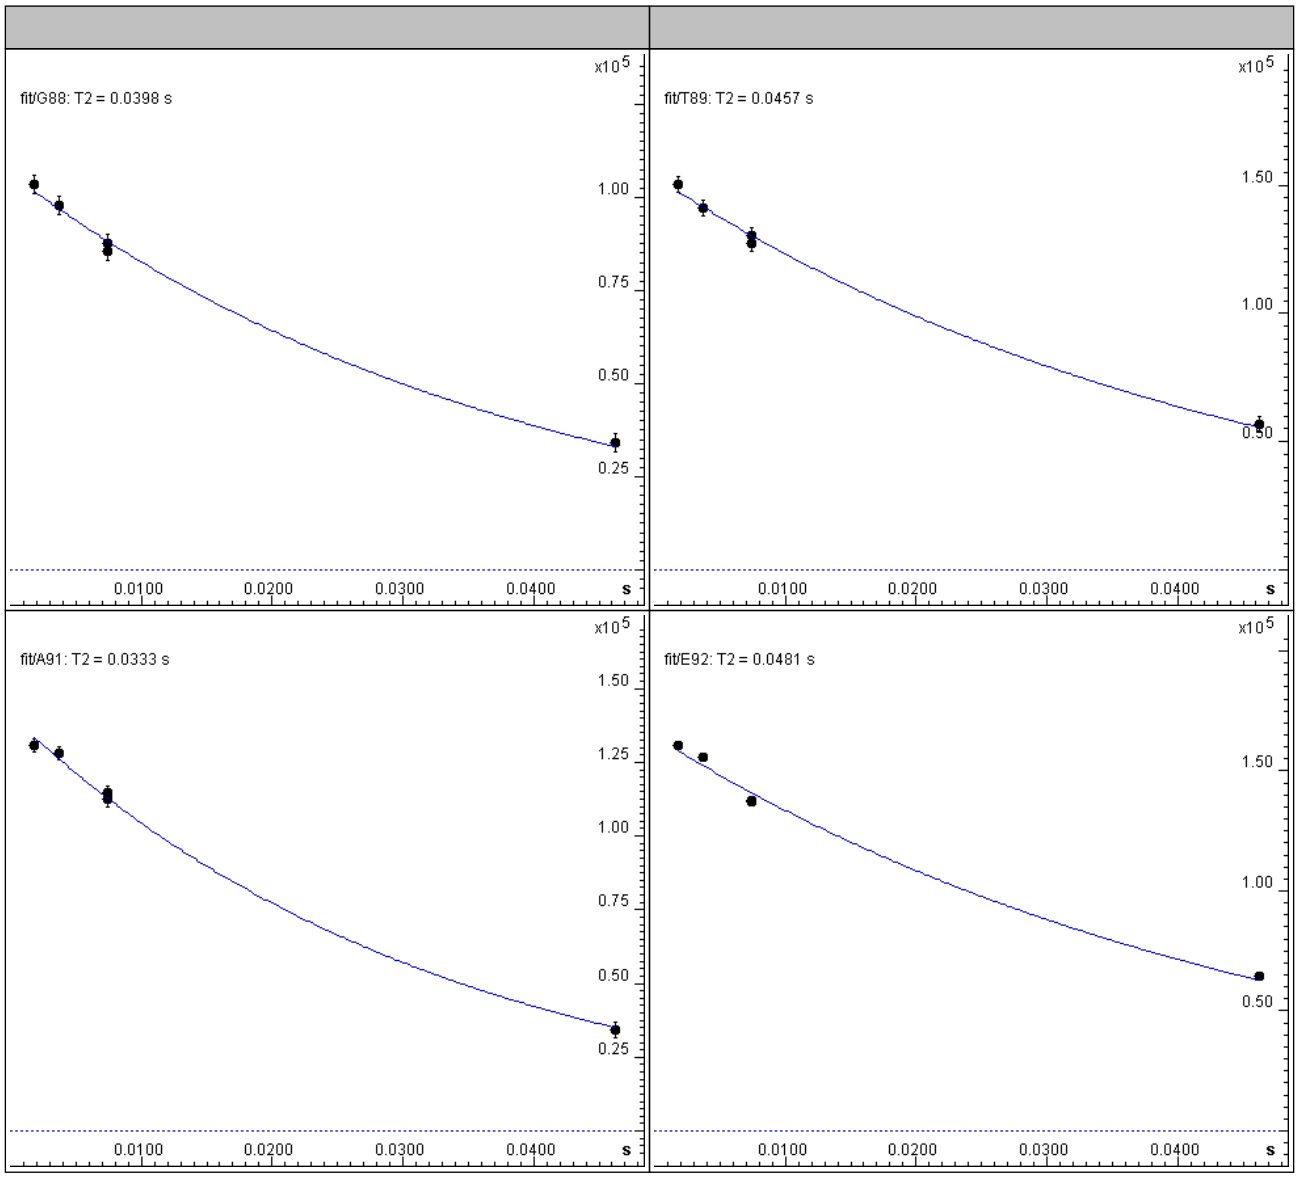

fit/S57: T2 = 0.0375 s
fit/I65: T2 = 0.0363 s
fit/T66: T2 = 0.0363 s
fit/N67: T2 = 0.0309 s
x10 5
0.0100
0.0200
0.0300
0.0400
s

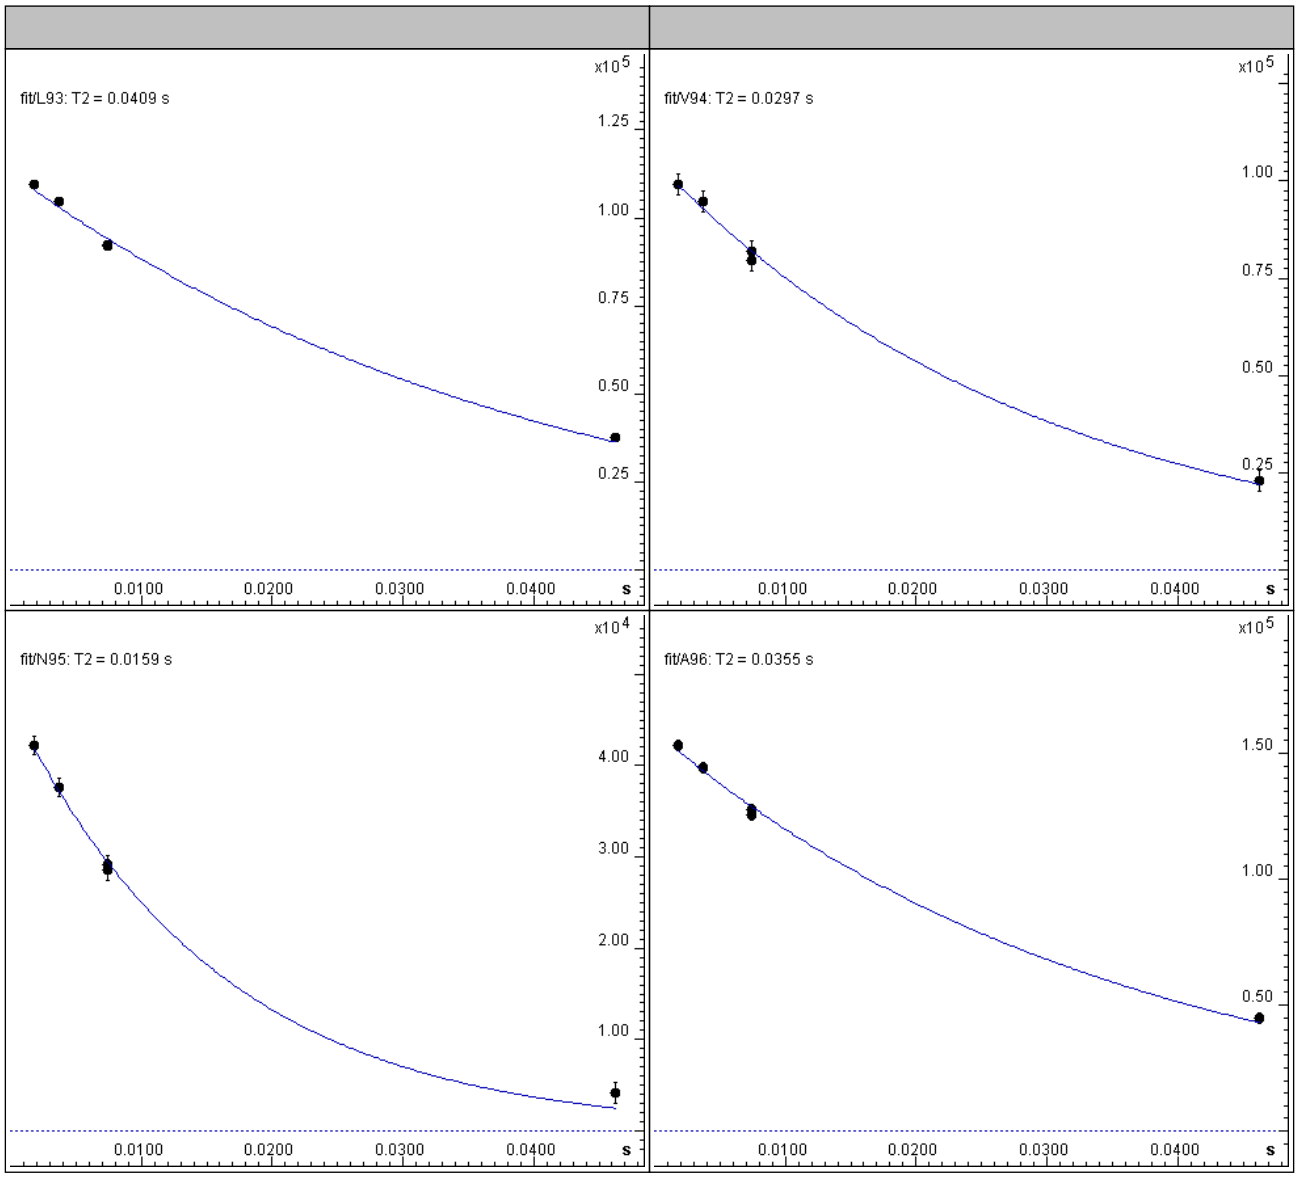

fit/A68: T2 = 0.0350 s
fit/G69: T2 = 0.0424 s
fit/W70: T2 = 0.0301 s
fit/N71: T2 = 0.0340 s
x10 5
1.25
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s

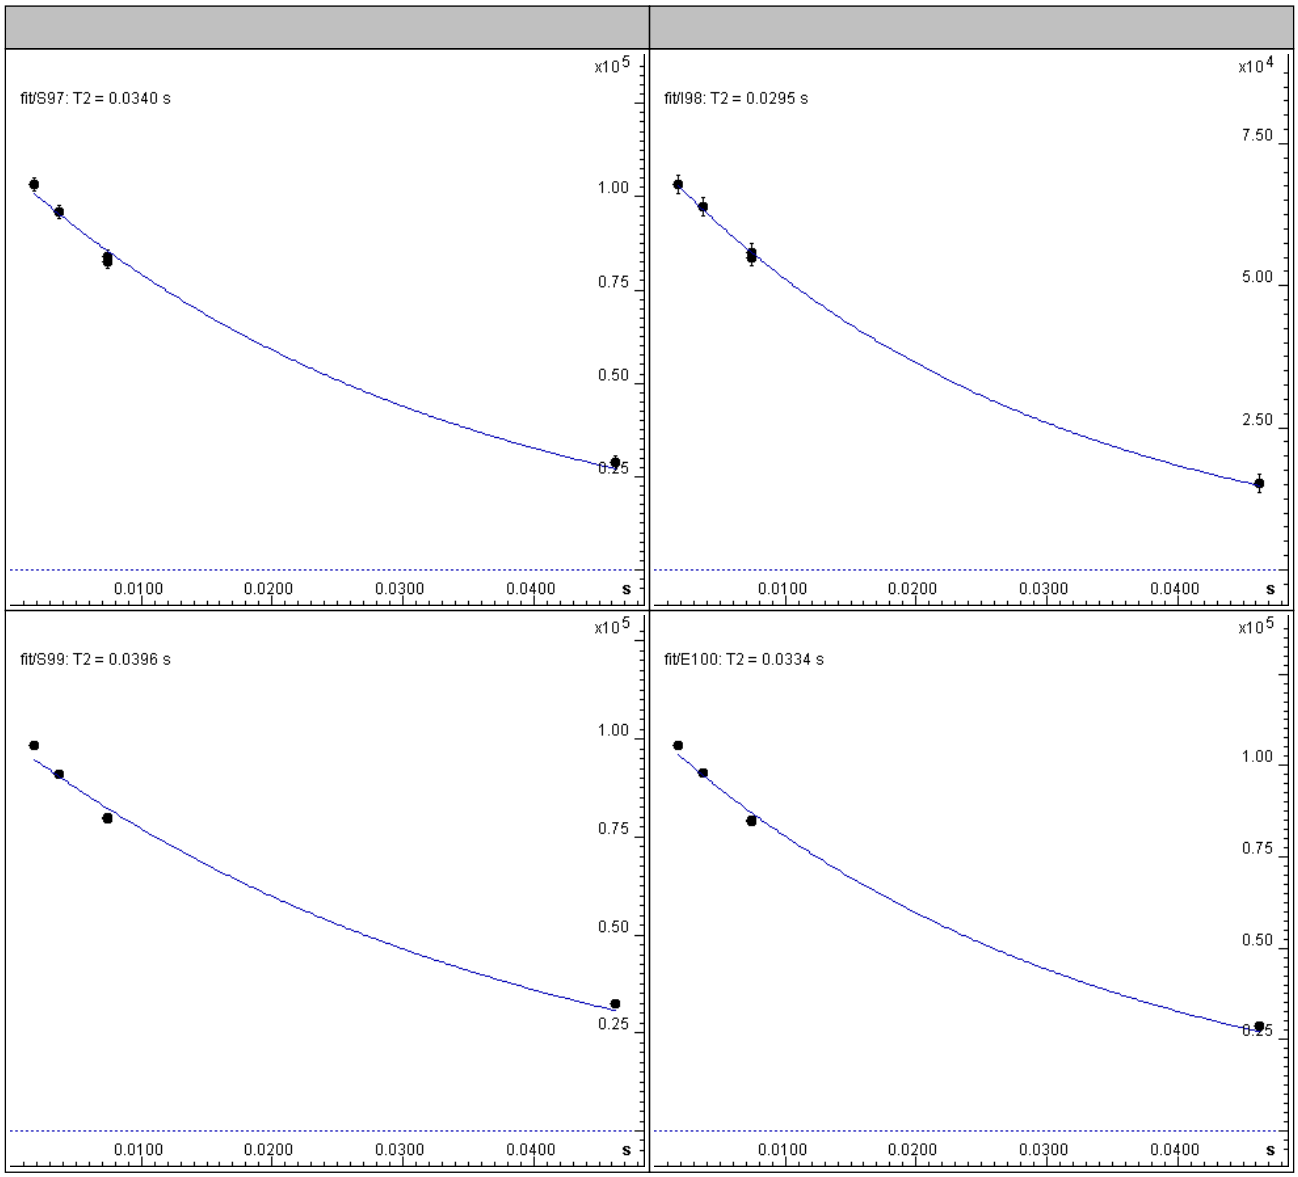

fit/E73: T2 = 0.0504 s
fit/I74: T2 = 0.0346 s
fit/G77: T2 = 0.0353 s
fit/G78: T2 = 0.0415 s
x10 5
0.0100
0.0200
0.0300
0.0400
s

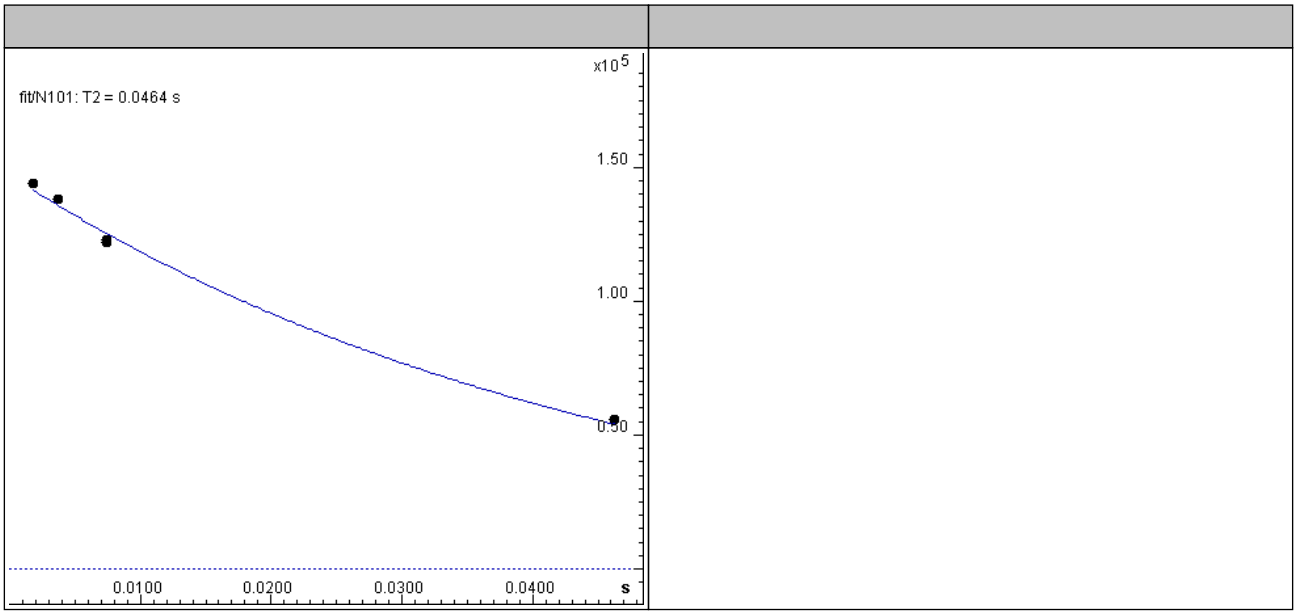

fit/S79: T2 = 0.0333 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/I80: T2 = 0.0398 s
x10 5
1.25
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/T81: T2 = 0.0259 s
x10 4
7.50
5.00
2.50
0.0100
0.0200
0.0300
0.0400
s
fit/I82: T2 = 0.0280 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s


fit/G83: T2 = 0.0158 s
x10 4
6.00
5.00
4.00
3.00
2.00
1.00
0.0100
0.0200
0.0300
0.0400
s
fit/A85: T2 = 0.0276 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/G86: T2 = 0.0371 s
x10 5
1.25
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/T87: T2 = 0.0444 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s


fit/G88: T2 = 0.0398 s
fit/T89: T2 = 0.0457 s
fit/A91: T2 = 0.0333 s
fit/E92: T2 = 0.0481 s
x10^5
0.0100
0.0200
0.0300
0.0400
s


fit/L93: T2 = 0.0409 s
x10 5
1.25
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/V94: T2 = 0.0297 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/N95: T2 = 0.0159 s
x10 4
4.00
3.00
2.00
1.00
0.0100
0.0200
0.0300
0.0400
s
fit/A96: T2 = 0.0355 s
x10 5
1.50
1.00
0.50
0.0100
0.0200
0.0300
0.0400
s


fit/S97: T2 = 0.0340 s
x10 5
1.00
0.75
0.50
0.25
0.0100
0.0200
0.0300
0.0400
s
fit/I98: T2 = 0.0295 s
x10 4
7.50
5.00
2.50
fit/S99: T2 = 0.0396 s
fit/E100: T2 = 0.0334 s


x10 5
fit/N101: T2 = 0.0464 s
1.50
1.00
0.50
0.0100
0.0200
0.0300
0.0400
s