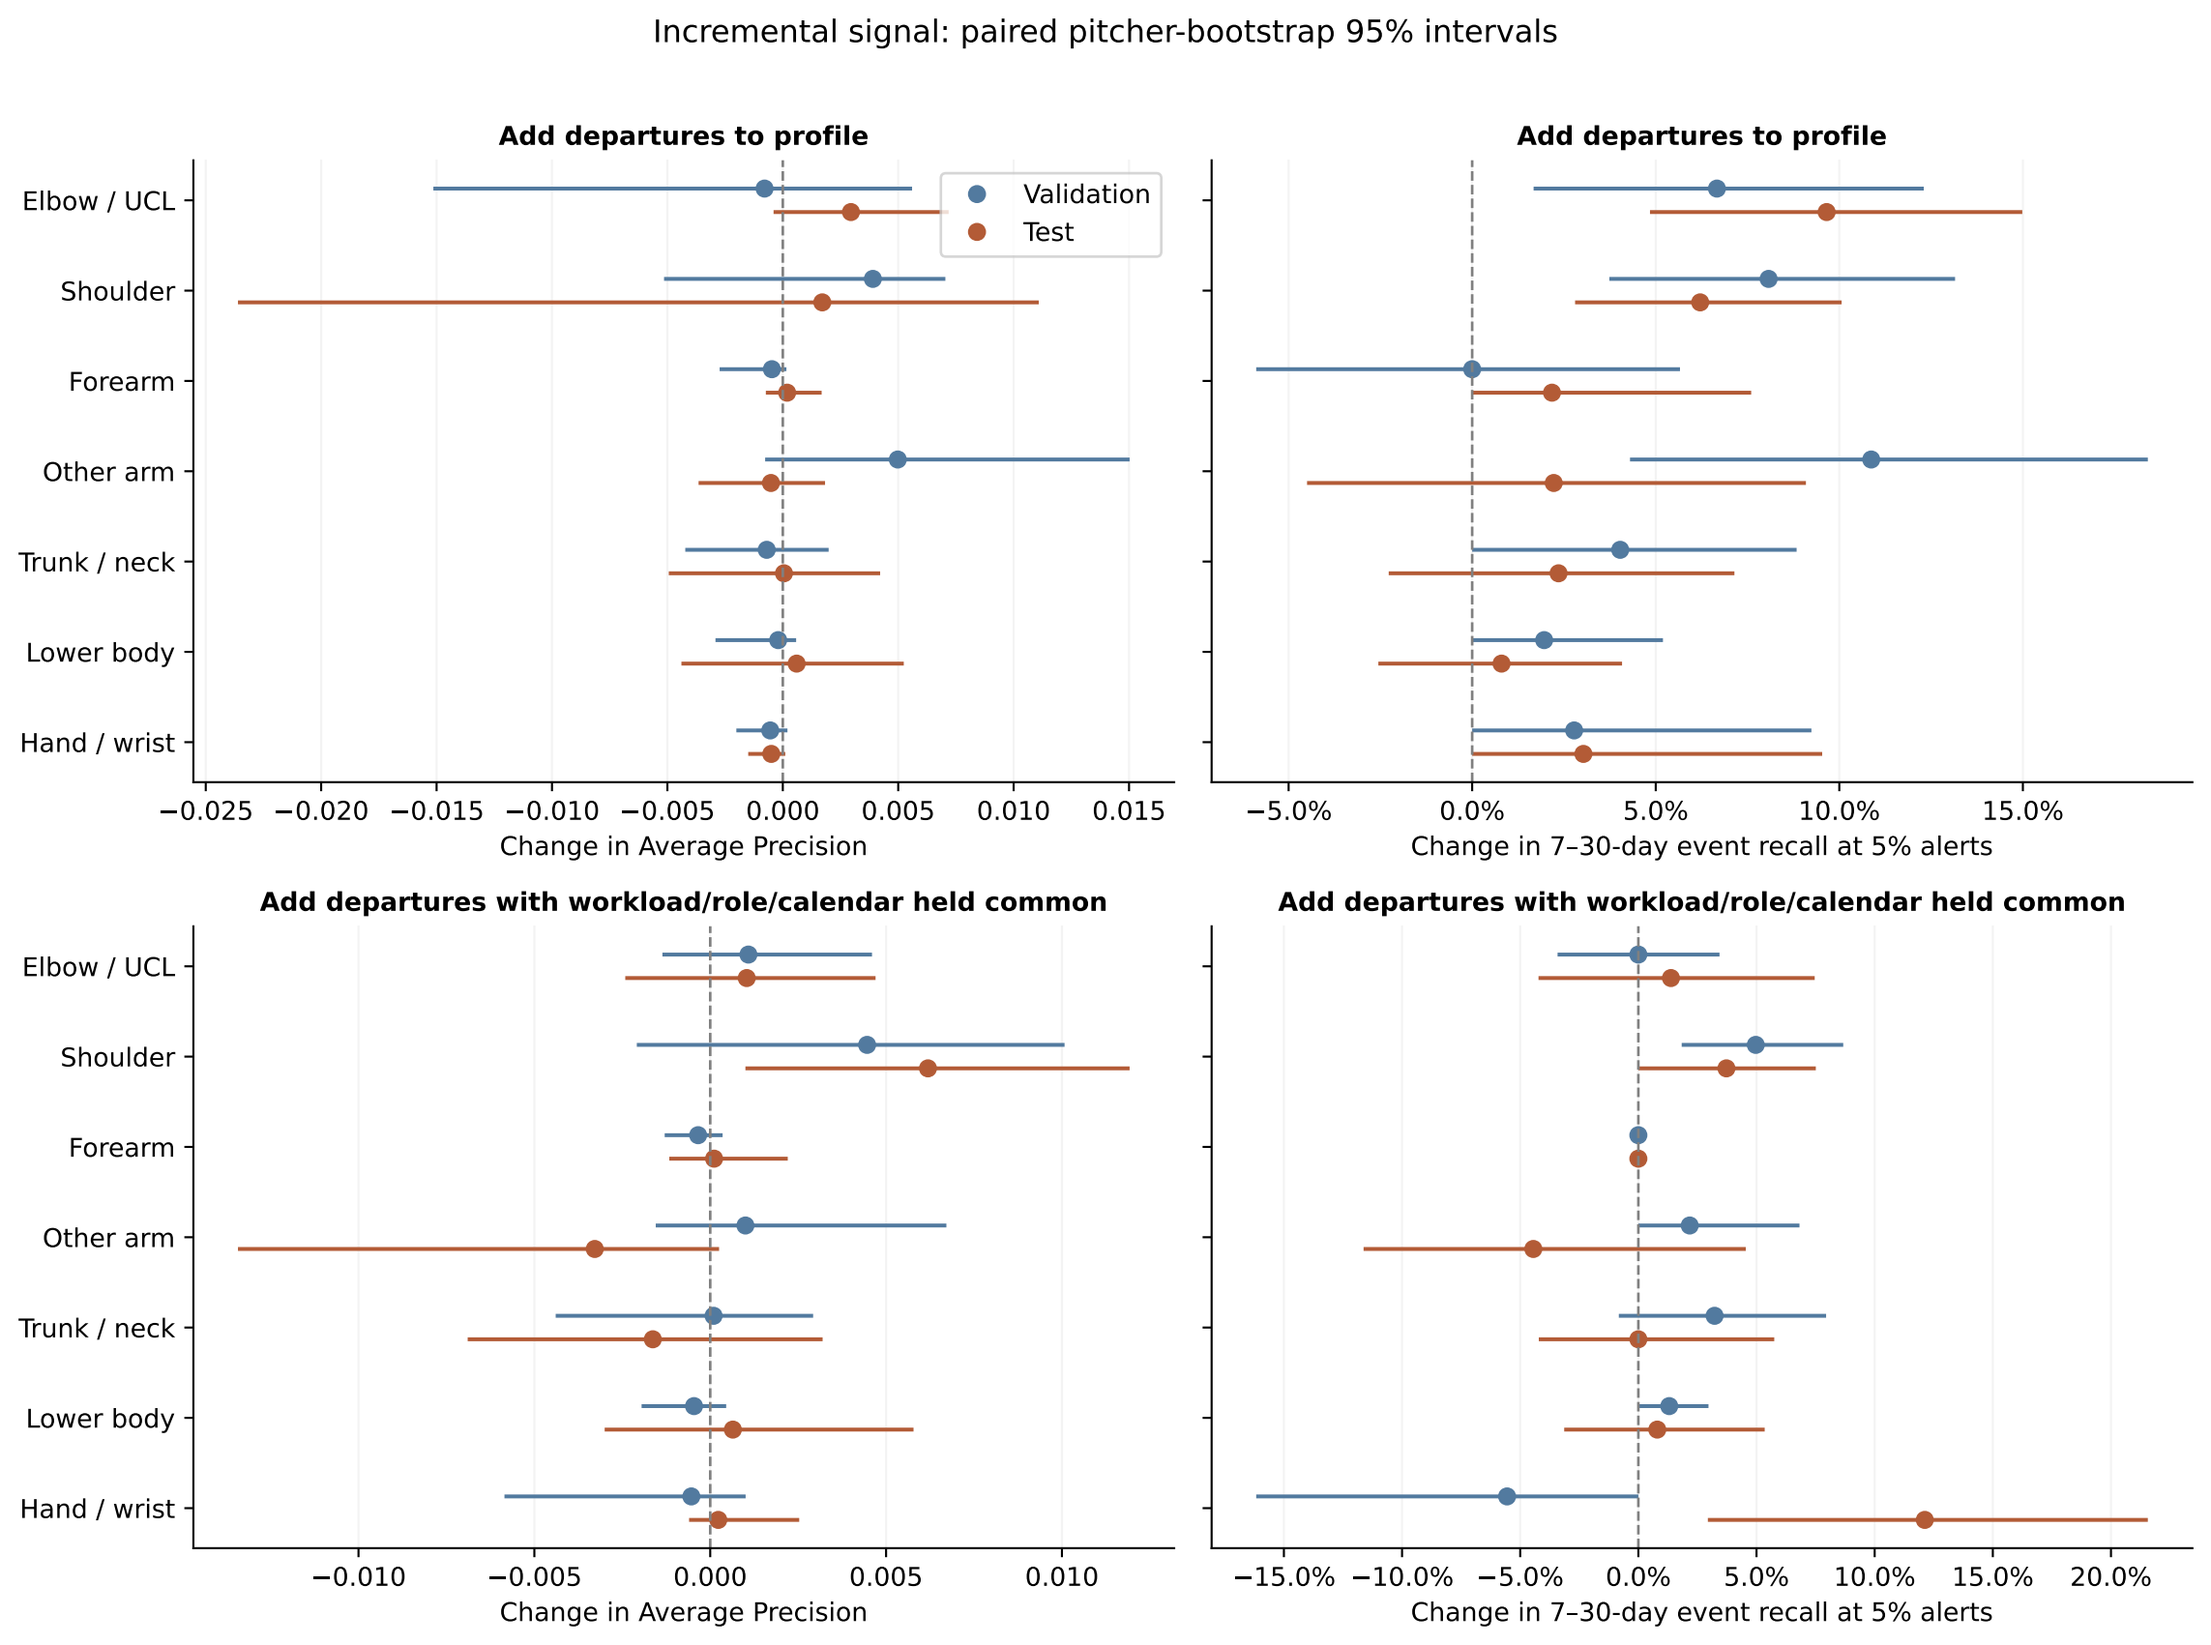
Incremental signal: paired pitcher-bootstrap 95% intervals
Add departures to profile
Validation
Test
Elbow / UCL
Shoulder
Forearm
Other arm
Trunk / neck
Lower body
Hand / wrist
−0.025 −0.020 −0.015 −0.010 −0.005 0.000 0.005 0.010 0.015
Change in Average Precision
Add departures to profile
−5.0% 0.0% 5.0% 10.0% 15.0%
Change in 7–30-day event recall at 5% alerts
Add departures with workload/role/calendar held common
Elbow / UCL
Shoulder
Forearm
Other arm
Trunk / neck
Lower body
Hand / wrist
−0.010 −0.005 0.000 0.005 0.010
Change in Average Precision
Add departures with workload/role/calendar held common
−15.0% −10.0% −5.0% 0.0% 5.0% 10.0% 15.0% 20.0%
Change in 7–30-day event recall at 5% alerts