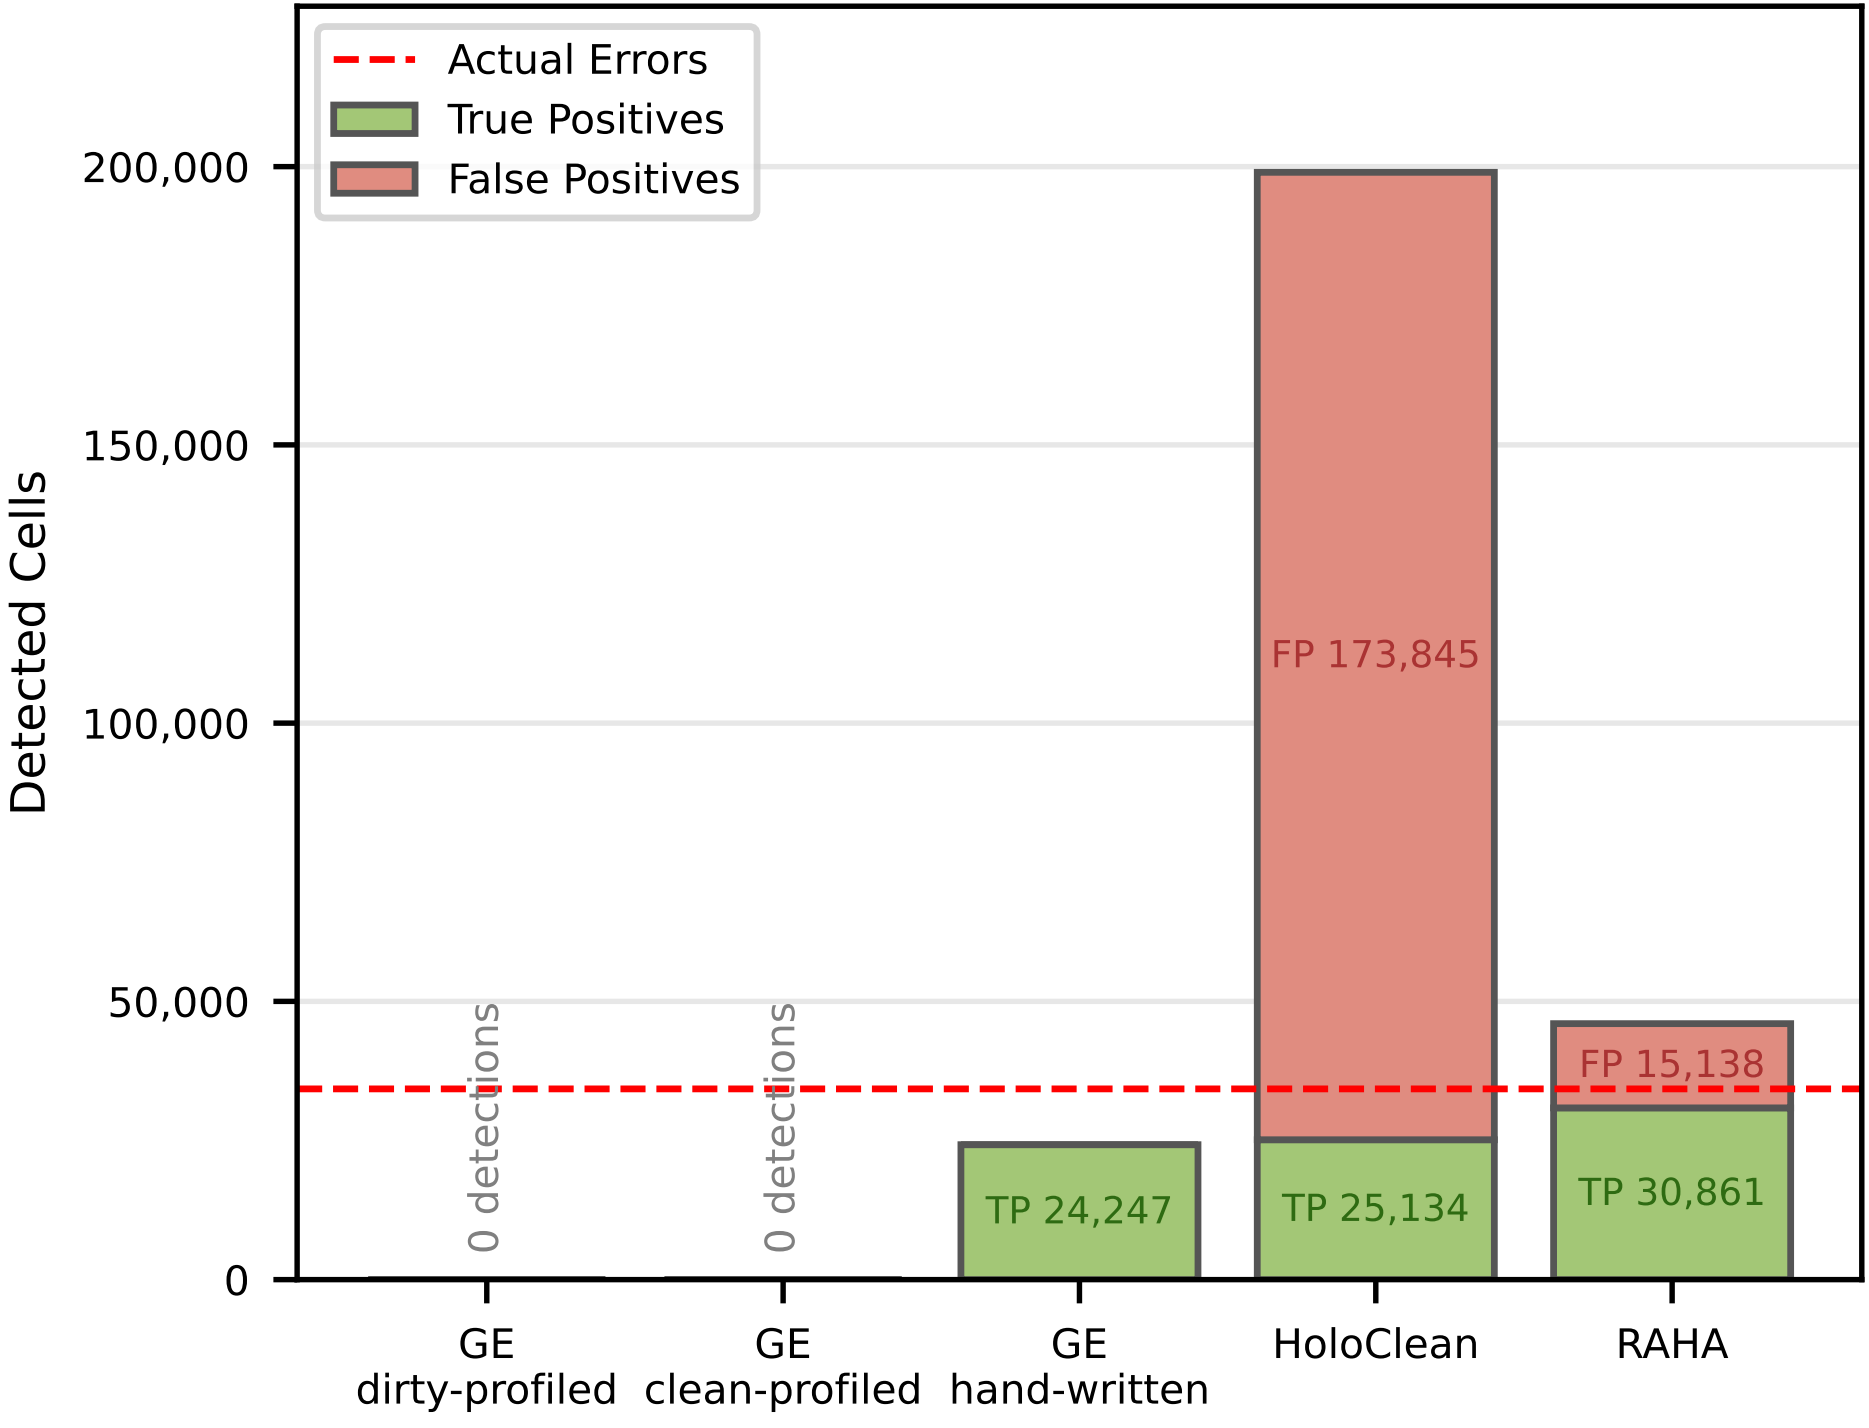
Actual Errors
True Positives
False Positives
Detected Cells
200,000
150,000
100,000
50,000
0
0 detections
0 detections
TP 24,247
FP 173,845
TP 25,134
FP 15,138
TP 30,861
GE
dirty-profiled
GE
clean-profiled
GE
hand-written
HoloClean
RAHA