


Username: FTIR Nicolet Summit-X
Report created: 18-02-2026 15:04 (GMT05:30)

Atanu_doped sample

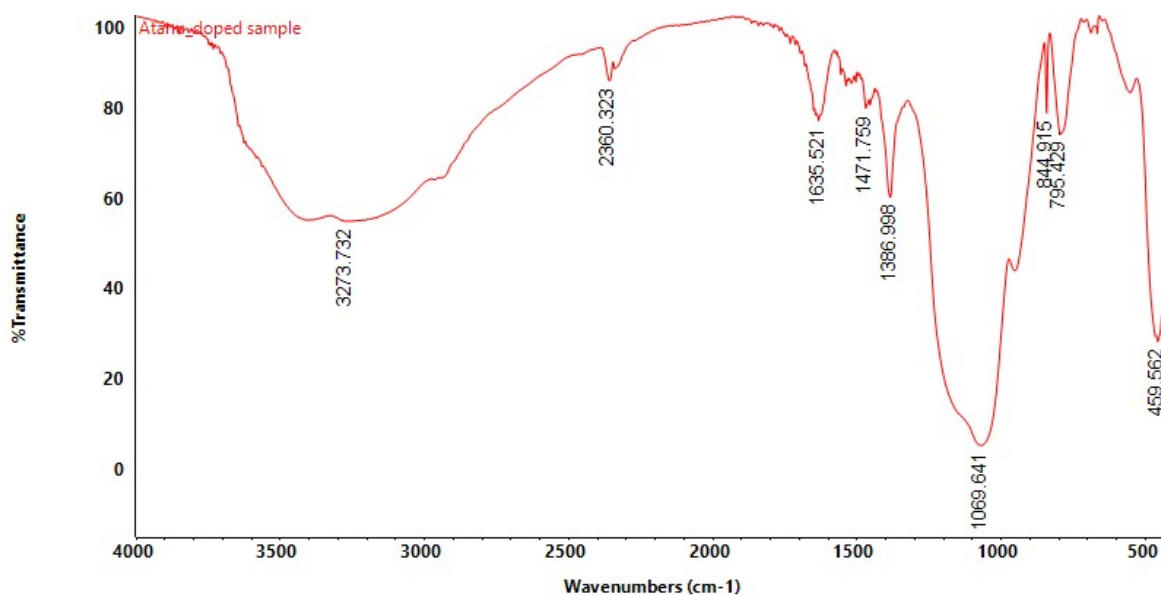

Title: Atanu_doped sample

Measurement date: 18-02-2026 14:58:02

Number of sample scans: 32

Number of background scans: 32

Instrument Serial: BGA2410563

Smart Accy: 40-5004562

Model: Nicolet Summit X

Source: IR

Detector: DTGS KBr

Smart Accessory Title: iD1 Transmission

Smart Accessory ID: 40-5004562

Crystal type: : None

Beamsplitter: KBr

Sample spacing: 1.0

Digitizer bits: 24

Optical velocity: 0.4747

Aperture: 100.0

Sample gain: 1.0

High pass filter: 20.0

Low pass filter: 11000.0

Comments: None

Regions:

Region 1: 3851.85-412.31

Threshold: 99.769

Sensitivity: 50.000

Position	Intensity
459.562	28.051
795.429	74.098
844.915	78.697
1069.641	5.081
1386.998	60.101
1471.759	79.763
1635.521	77.074
2360.323	85.936
3273.732	54.748