


Username: FTIR Nicolet Summit-X
Report created: 18-02-2026 14:49 (GMT05:30)

basudev roy ref

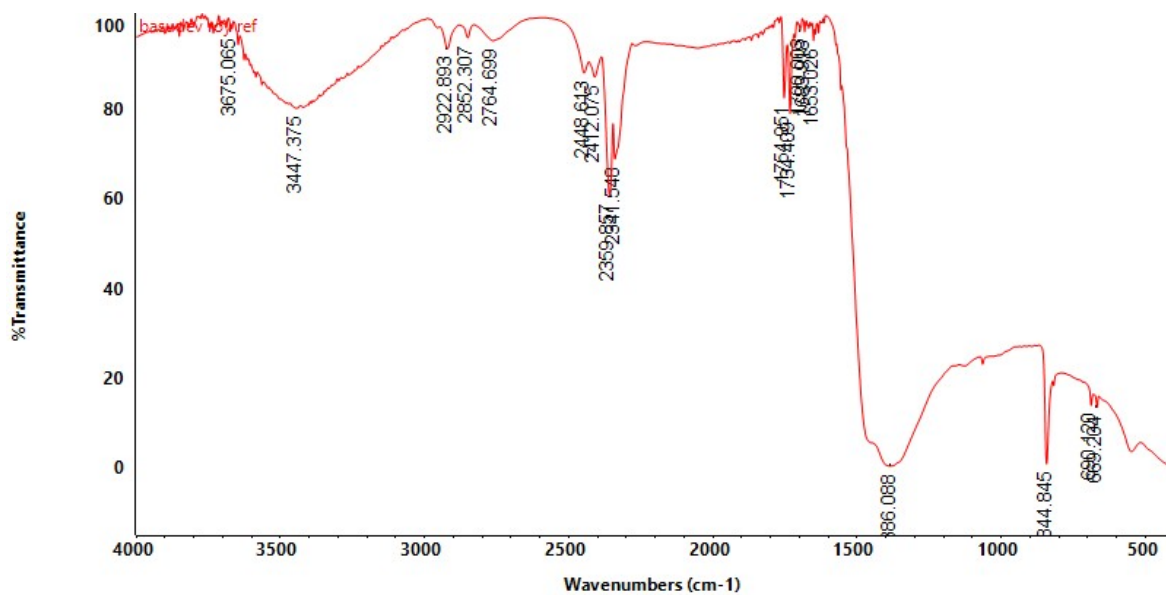

Regions:

Region 1: 3732.74-456.06
Threshold: 99.767
Sensitivity: 60.000

Title: basudev roy ref
Measurement date: 18-02-2026 14:45:53
Number of sample scans: 32
Number of background scans: 32
Instrument Serial: BGA2410563
Smart Accy: 40-5004562
Model: Nicolet Summit X
Source: IR
Detector: DTGS KBr
Smart Accessory Title: iD1 Transmission
Smart Accessory ID: 40-5004562
Crystal type: : None
Beamsplitter: KBr
Sample spacing: 1.0
Digitizer bits: 24
Optical velocity: 0.4747
Aperture: 100.0
Sample gain: 1.0
High pass filter: 20.0
Low pass filter: 11000.0
Comments: None

Position	Intensity
669.204	13.180
690.120	13.623
844.845	0.536
1386.088	0.026
1653.026	95.158
1683.918	97.136
1700.003	97.335
1734.409	78.804
1754.951	82.344
2341.548	68.704
2359.857	60.576
2412.075	87.067
2448.613	87.961
2764.699	95.159
2852.307	95.849
2922.893	93.382
3447.375	80.024
3675.065	97.275