


False Positive Analysis — Test Set (South America, RF)
Top-5% risk zone: 283,214 true positives / 2,101,563 false positives precision=0.119

True Positives
(high-risk → actually became protected)



False Positives
(high-risk → NOT protected in test window)

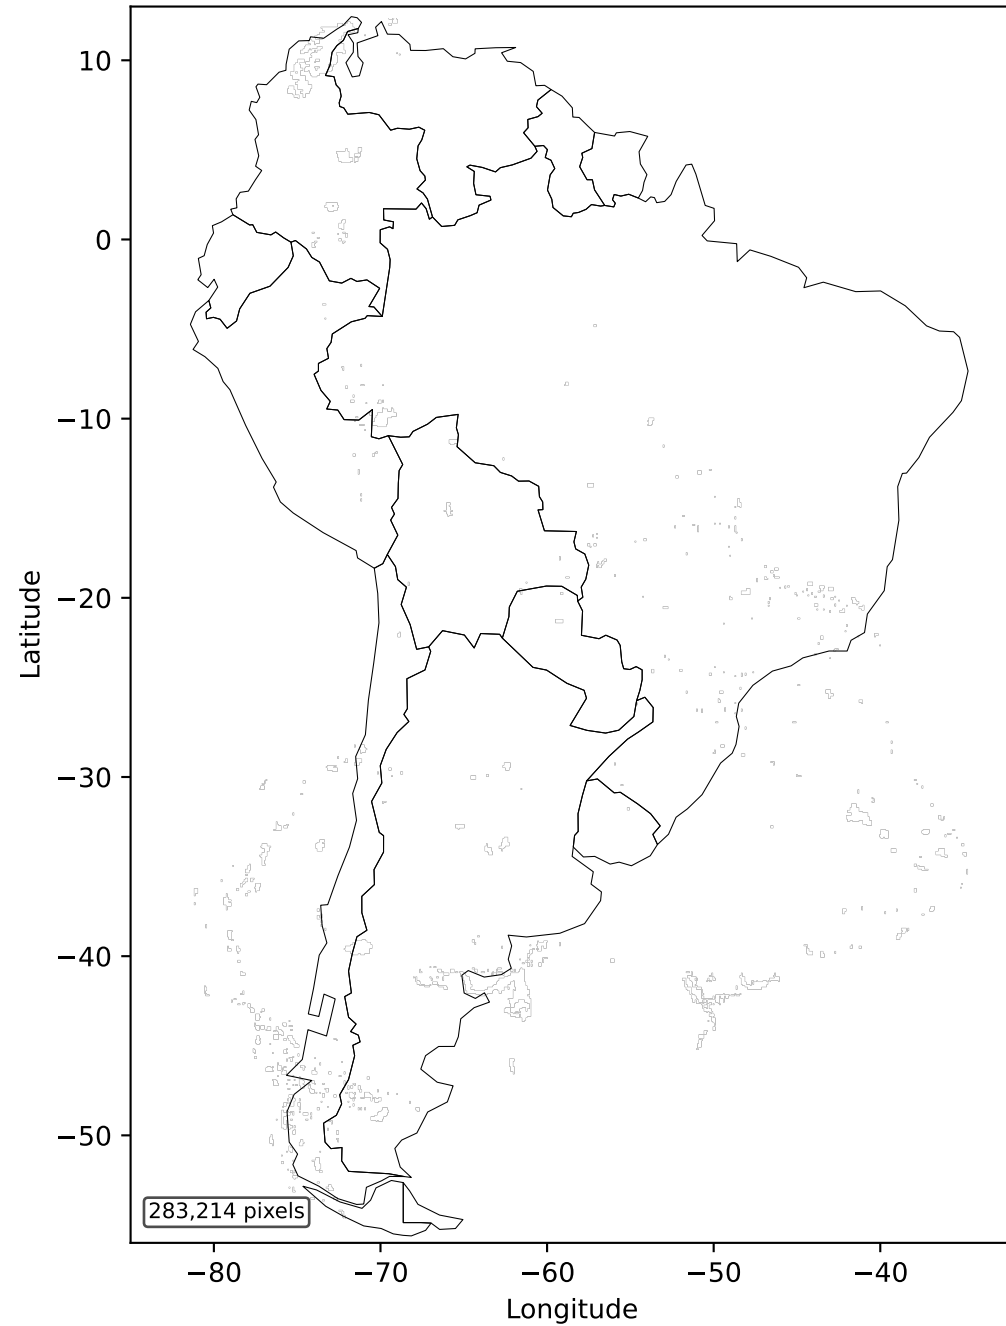