

MPADMIN 2/18/2015 11:25:01 AM	User: Institution: Software: Date:	LSRFortessa H657427C2001 HT5 HT5	Cytometer: Cytometer Name: Serial Number: Input Device: Window Extension:
----------------------------------	---	---	---


ESC (488nm) Blue Laser

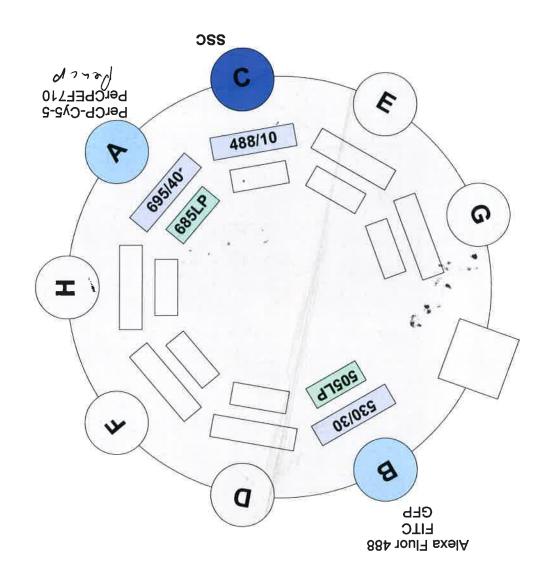



5%C 40.4 47.41

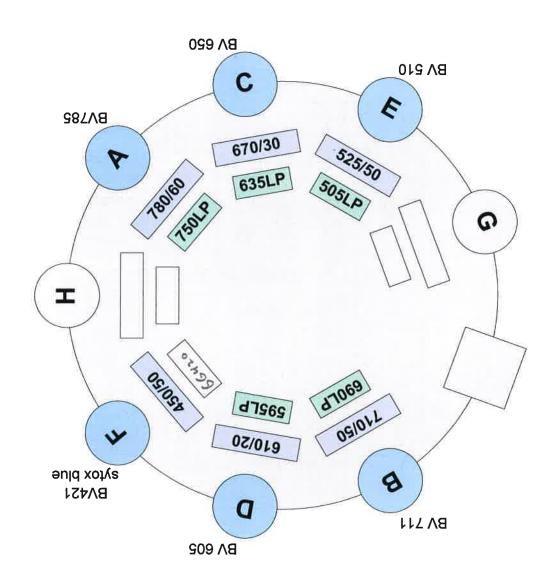

Violet Laser (405nm)

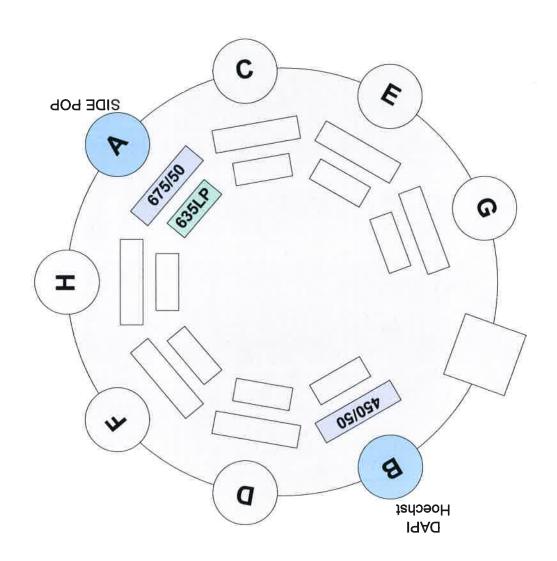

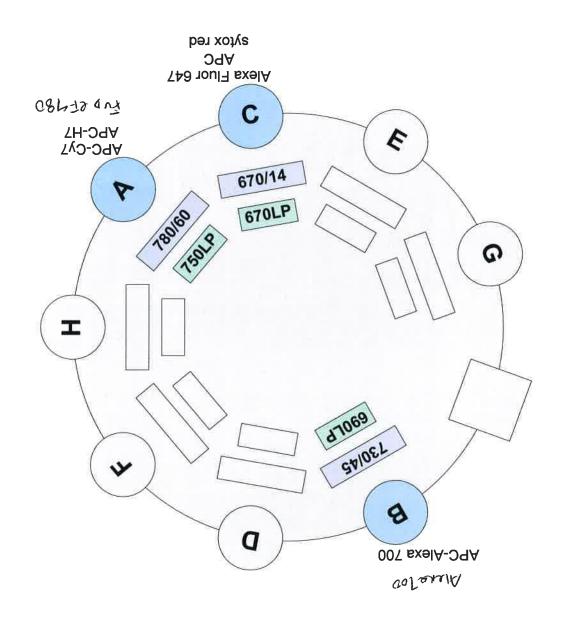

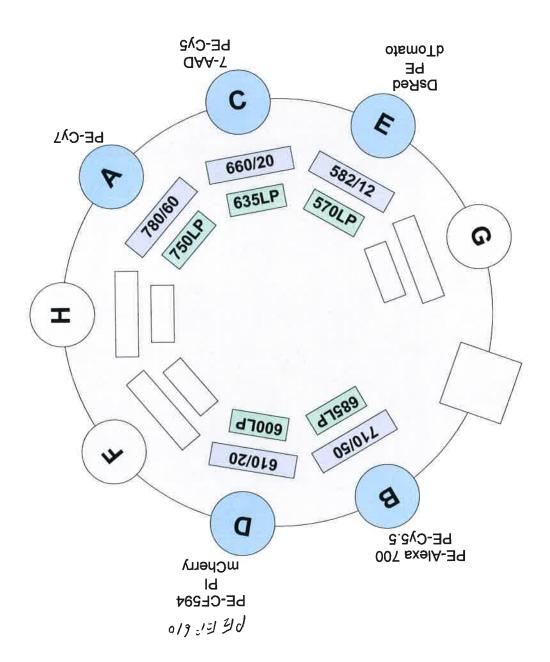

YG Laser (561nm)