
Structure indication and technical parameters

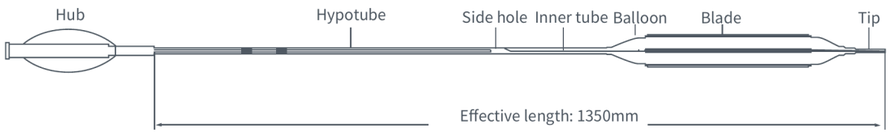

1. Adapted guiding catheter: Minimum guiding catheter 1.8mm/6F
2. Adapted guiding wire:0.36mm/0.014inch
3. Effective length of the catheter:1350mm
4. Marker location:Both ends of the balloon

Specification

Diameter/mm	length/mm			number of blades
	5	10	15	
2.0	√	√	√	3
2.25	√	√	√	
2.5	√	√	√	
2.75	√	√	√	
3.0	√	√	√	
3.25	√	√	√	
3.5	√	√	√	4
3.75	√	√	√	
4.0	√	√	√	

Compliance table

Nominal pressure Rated Burst pressure

Diameter (mm)	Pressure (atm)								
	4	5	6	7	8	9	10	11	12
2.0	1.90	1.95	**2.00**	2.04	2.08	2.12	2.16	2.20	**2.25**
2.25	2.15	2.20	**2.25**	2.29	2.33	2.37	2.41	2.45	**2.50**
2.5	2.40	2.45	**2.50**	2.54	2.58	2.62	2.66	2.70	**2.75**
2.75	2.65	2.70	**2.75**	2.79	2.83	2.87	2.91	2.95	**3.00**
3.0	2.90	2.95	**3.00**	3.04	3.08	3.12	3.16	3.20	**3.25**
3.25	3.15	3.20	**3.25**	3.29	3.33	3.37	3.41	3.45	**3.50**
3.5	3.40	3.45	**3.50**	3.54	3.58	3.62	3.66	3.70	**3.75**
3.75	3.65	3.70	**3.75**	3.79	3.83	3.87	3.91	3.95	**4.00**
4.0	3.90	3.95	**4.00**	4.04	4.08	4.12	4.16	4.20	**4.25**

LEPU MEDICAL

Lepu Medical Technology (Beijing) Co.,LTD.

No.37 Chaoqian Road,Changping District, Beijing, China, 102200
Tel:+86-10-80120666
Email:lepuservice@lepumedical.com
Web:en.lepumedical.com

SELLMED BRASIL
PRODUTOS QUE SALVAM VIDAS

LEPU MEDICAL

Vesscide™

Cutting Balloon System

Essential weapon for PCI pretreatment

SELLMED BRASIL
PRODUTOS QUE SALVAM VIDAS




Product Features

Segmented Microsurgical blades Design

- Sharp and anti-friction blades, balance cutting force and flexibility
- Blades' Working height is only 0.13mm, which could avoid blood vessel perforation
- Pre-made longitudinal neat blades, which could reduce the risk of intimal disordered tearing

Semi-compliant balloon

- Improve crossability
- Optimize retraction

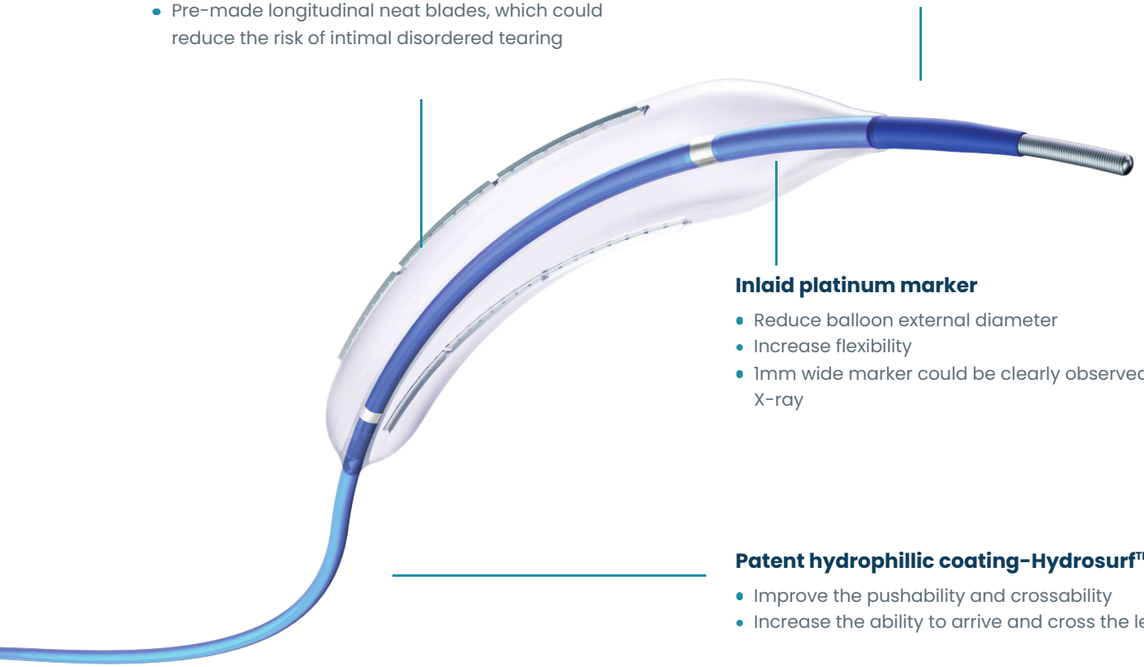

Inlaid platinum marker

- Reduce balloon external diameter
- Increase flexibility
- 1mm wide marker could be clearly observed under X-ray

Patent hydrophillic coating-Hydrosurf™

- Improve the pushability and crossability
- Increase the ability to arrive and cross the lession


Unique advantages

Dilated under low pressure

Can benefit from vascular lumen

Change the compliance of the lession

Reduce the axial migration of plaque, and decrease lumen elastic retraction



Cutting the lession neatly and orderly

Reduce the risk of irregular dissection and acute occlusion


Anchoring the lession precisely

Avoid balloon slipping, and squeeze plaque by larger area

Vesscide™

Indications

The cutting balloon system is indicated to be applied for patients with atherosclerotic plaques in the coronary arteries that need to be cut.

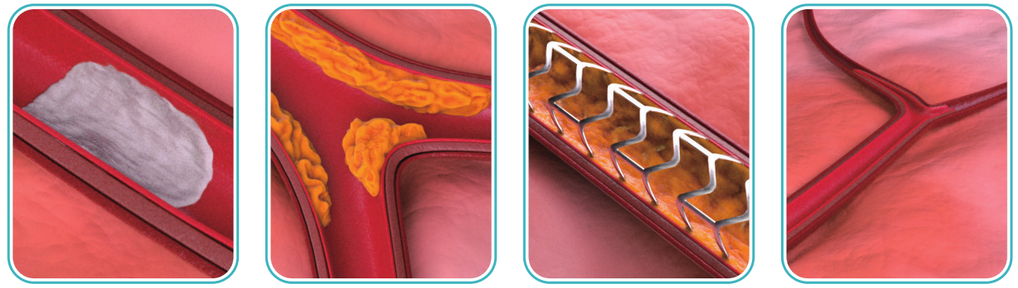

Calcified lesions | Ostia lession and bifurcation lesions | Stent restenosis | Small vessel lessions

References:

1.Weiming Wang,Yong Huo,Junbo Ge,<the consensus of Chinese specialis in treatment of calcified coronary artery lession > [J],Chinese Journal of Interventional Cardiology.2014(22):69-73.

2.The specialist team of <the consensus of Chinese specialis in the clinical application of drug coated balloon>,<the consensus of Chinese specialis in the clinical application of drug coated balloon>[J],Chinese Journal of Interventional Cardiology.2016(2):61-67.

3.Yalin Han,<the consensus of Chinese specialis in the clinical application of coronary bioabsorb stent >[J], Chinese Journal of cardiovascular disease.2020.(5):350-358.

Performance tips

Can be expanded repeatedly, do not reverse the catheter between two expansions

Choosing specification	Balloon dilatation	Balloon withdraw
Diameter: The ratio of cutting balloon and blood vessel is better to be 0.8~1.0:1 **Length:** choosing according to the lession length, the pushability of shorter balloon is more excellent.	Slowly dilated the balloon to 6atm or nominal pressure by 1atm/5s, and keep pressure by 20s. Do not repeatly dilated the same lession segment.	Slowly depressuring the balloon to vacuum by 1atm/5s, and withdraw into the guiding catheter afterwards. Slowly depressuring could help getting the best refold result.

SELLMED BRASIL
PRODUTOS QUE SALVAM VIDAS