Vesselin®
DRUG COATED CORONARY BALLOON CATHETER

Specification

Diameter /mm	Length / mm										
	9	12	14	16	18	20	24	28	31	35	38
2.0	LPCDB 20009	LPCDB 20012	LPCDB 20014	LPCDB 20016	LPCDB 20018	LPCDB 20020	LPCDB 20024	LPCDB 20028	LPCDB 20031	LPCDB 20035	LPCDB 20038
2.5	LPCDB 25009	LPCDB 25012	LPCDB 25014	LPCDB 25016	LPCDB 25018	LPCDB 25020	LPCDB 25024	LPCDB 25028	LPCDB 25031	LPCDB 25035	LPCDB 25038
2.75	LPCDB 27009	LPCDB 27012	LPCDB 27014	LPCDB 27016	LPCDB 27018	LPCDB 27020	LPCDB 27024	LPCDB 27028	LPCDB 27031	LPCDB 27035	LPCDB 27038
3.0	/	LPCDB 30012	/	LPCDB 30016	LPCDB 30018	LPCDB 30020	LPCDB 30024	LPCDB 30028	LPCDB 30031	LPCDB 30035	LPCDB 30038
3.5	/	LPCDB 35012	/	LPCDB 35016	LPCDB 35018	LPCDB 35020	LPCDB 35024	LPCDB 35028	LPCDB 35031	LPCDB 35035	LPCDB 35038
4.0	/	LPCDB 40012	/	LPCDB 40016	LPCDB 40018	LPCDB 40020	LPCDB 40024	LPCDB 40028	LPCDB 40031	LPCDB 40035	LPCDB 40038

Balloon compliance

Nominal pressure Burst Pressure

Diameter /mm	Expansion pressure （atm）										
	203 (2)	405 (4)	608 (6)	810 (8)	1013 (10)	1216 (12)	1418 (14)	1621 (16)	1824 (18)	2027 (20)	2229 (22)
2.00	1.86	1.91	1.96	2.00	2.06	2.12	2.18	2.23	2.29	2.35	2.41
2.50	2.35	2.40	2.45	2.50	2.56	2.62	2.68	2.75	2.81	2.86	2.92
2.75	2.60	2.67	2.72	2.75	2.82	2.88	2.94	3.00	30.6	3.12	3.18
3.00	2.84	2.89	2.95	3.00	3.06	3.12	3.18	3.25	3.30	3.36	3.43
3.50	3.39	3.44	3.50	3.56	3.62	3.68	3.74	3.81	3.88	3.95	4.00
4.00	3.88	3.94	4.00	4.06	4.12	4.19	4.26	4.33	4.40	4.47	4.55

LEPU MEDICAL TECHNOLOGY (BEIJING) CO., LTD.


No.37 Chaoqian Road, Changping District, Beijing 102200, P.R. China
Tel:+86-10-80120666
Fax:+86-10-80120600
Website: https://en.lepumedical.com/

SELLMED BRASIL
PRODUTOS QUE SALVAM VIDAS

LEPU MEDICAL

Vesselin®

DRUG COATED CORONARY BALLOON CATHETER

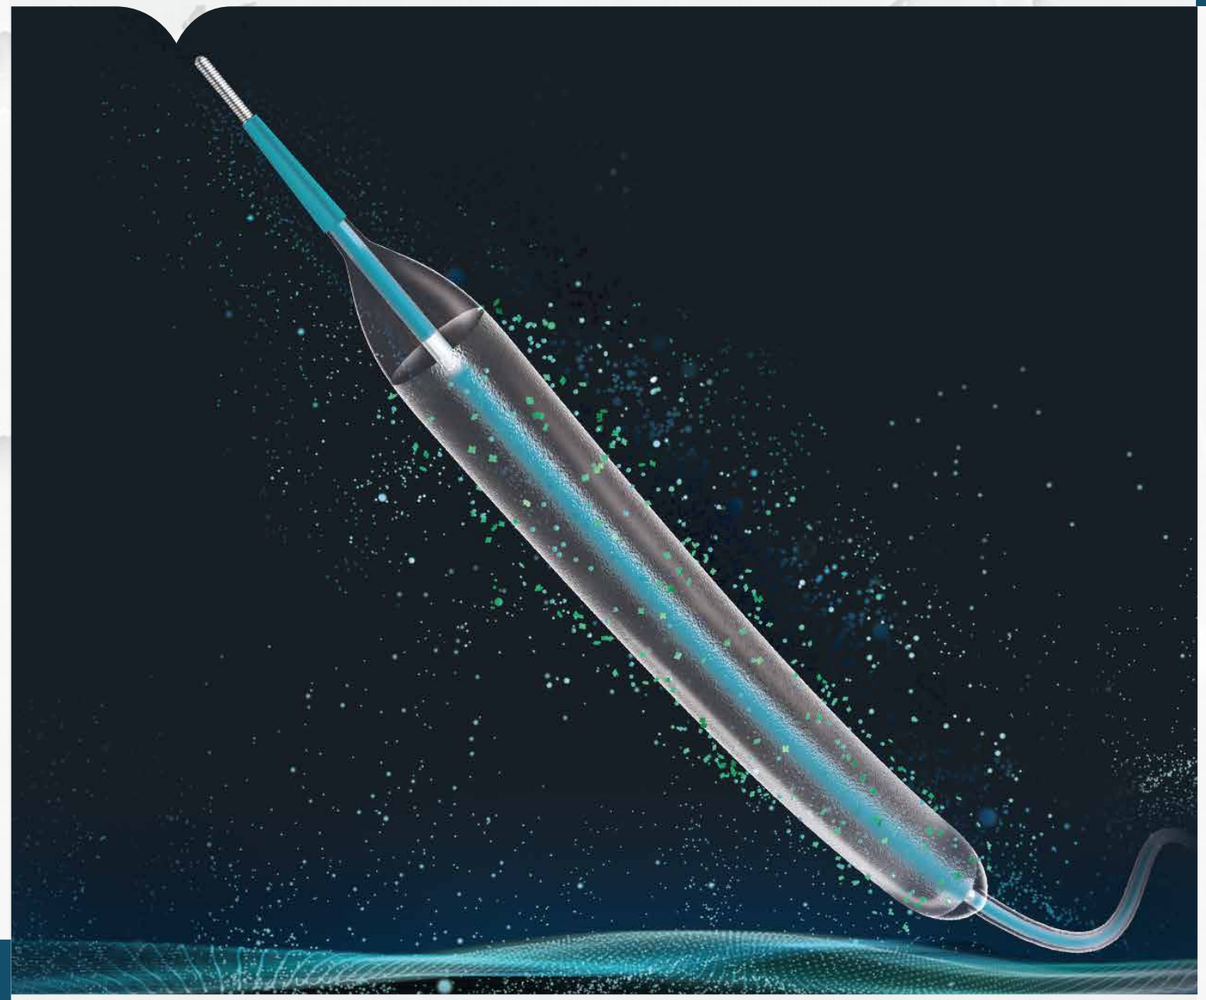




LEPU MEDICAL TECHNOLOGY (BEIJING) CO., LTD.

BALLOON STRUCTURE FEATURES

Drug Coating


Coating with Active Pharmaceutical Ingredients grade urea, provide better biocompatibility, facilitate drug releasing effectively. Drug release rate in vivo achieves more than 90%.


Suitable particle size at 2-3μm, enables long term efficacy and low embolism risk



Drug

Paclitaxel loaded with drug dose at 3μg/mm², inhibits restenosis continuously



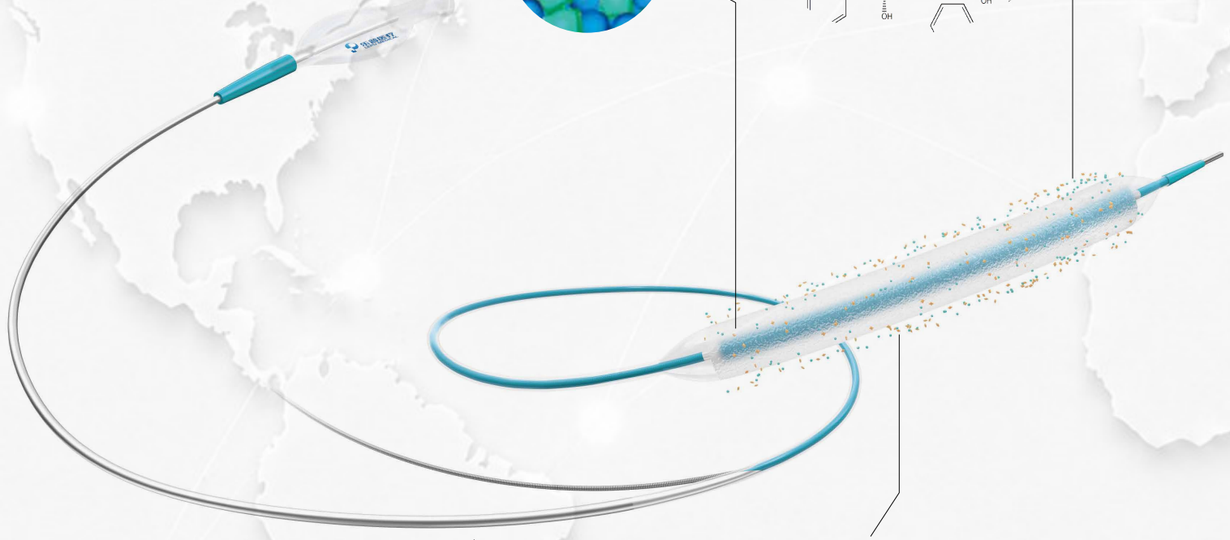

Delivery System

Spiral cut hypotube design, strengthens the transition section, brings optimized deliver-ability for transition.

Materials

Improved PEBAX material, lower crossing profile guarantees higher flexibility and enhanced crossability.


TECHNIQUE PARAMETERS

Balloon Material: PEBAX
Effective length: 1350mm
Distal Shaft O.D.: 2.7F

Balloon crossing profile: 0.026" - 0.035"
Guiding catheter compatibility: 5F and above
Guide wire compatibility: 0.014"

Safe and effective Drug dose, drug releasing keeps continuously and stably


The effective drug concentration keeps at least 28 days, and inhibits Intimal hyperplasia in long term.

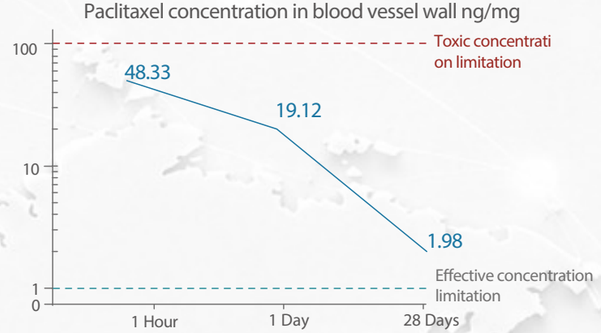


References: Juan F. Granada. The Technical Evolution of Local Drug Delivery: Implications for the Clinical Adoption of Coronary DCB. TCT 2015

Balanced safety and effectiveness

Compared with the control group, no significant difference for late lumen loss in segment in 9 months, thrombosis and TLF in 12 months .(TLF: Target lesion failure)

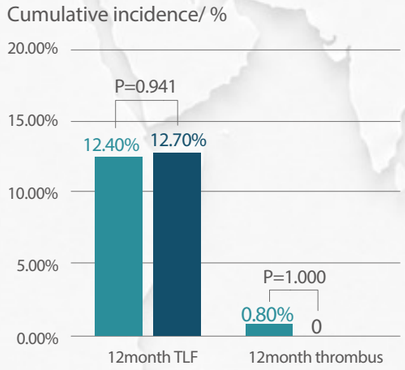

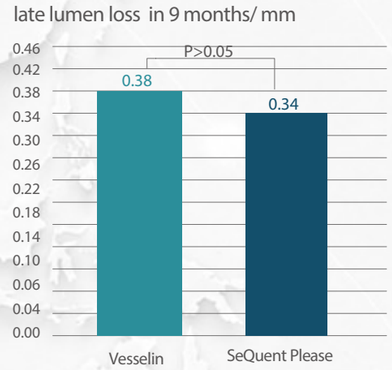

Drug balloon manipulation procedures instruction

Lesion prepare
Pre-dilatation with ordinary balloon, balloon/artery diameter ratio is 0.8-1.0, dilatation pressure > standard pressure

Angiographic results are acceptable,
No dissection or only type A or B dissection, TIMI blood flow class III, residual stenosis ≤ 30%

DCB treatment
CB distal part and proximal part should be 2-3mm longer than the pre-dilatation area.
Balloon/artery diameter ratio is 0.8-1.0
Apply dilatation at 7atm pressure for 30-60s.

DAPT
Only DCB: 1-3 months
BMS-ISR:1-3months
DES-ISR:duation depends on DES, but at least 1-3 months
Spot-BMS&DCB:3 months

SELLMED BRASIL
PRODUTOS QUE SALVAM VIDAS