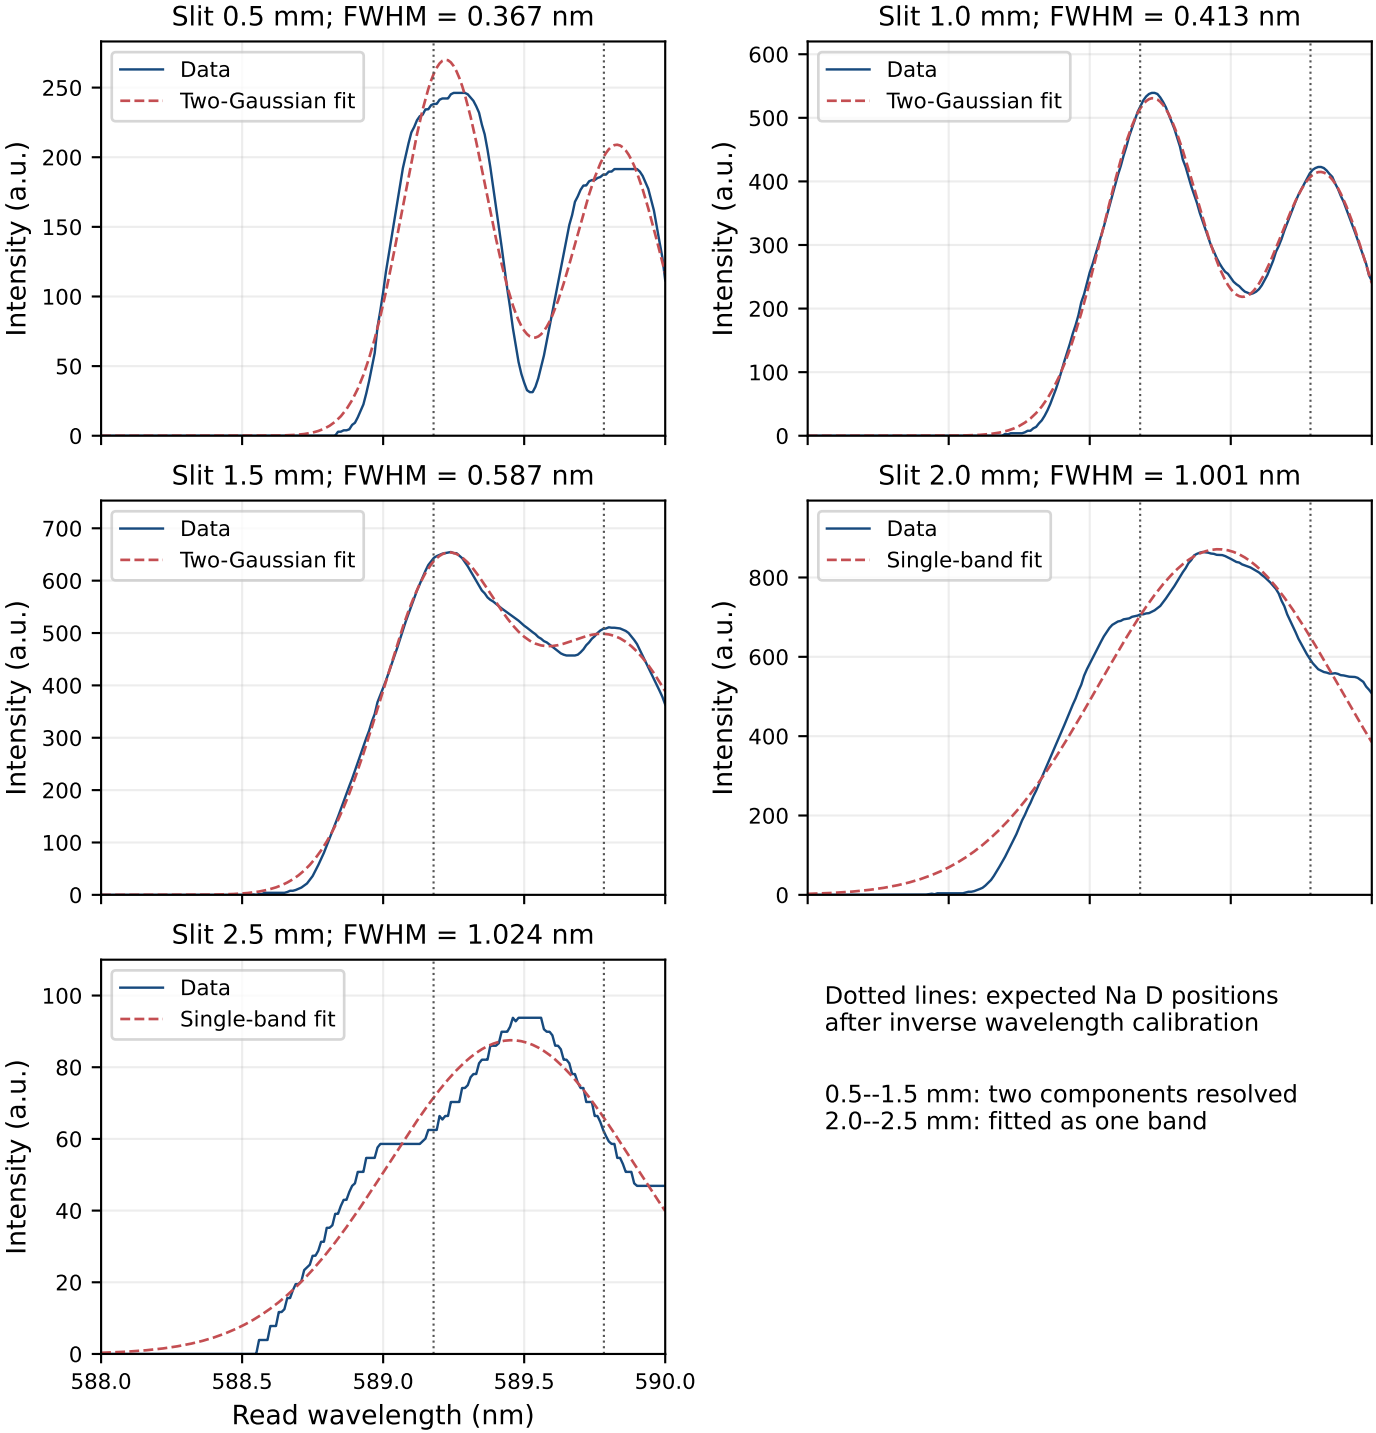

Dotted lines: expected Na D positions
after inverse wavelength calibration

0.5--1.5 mm: two components resolved
2.0--2.5 mm: fitted as one band