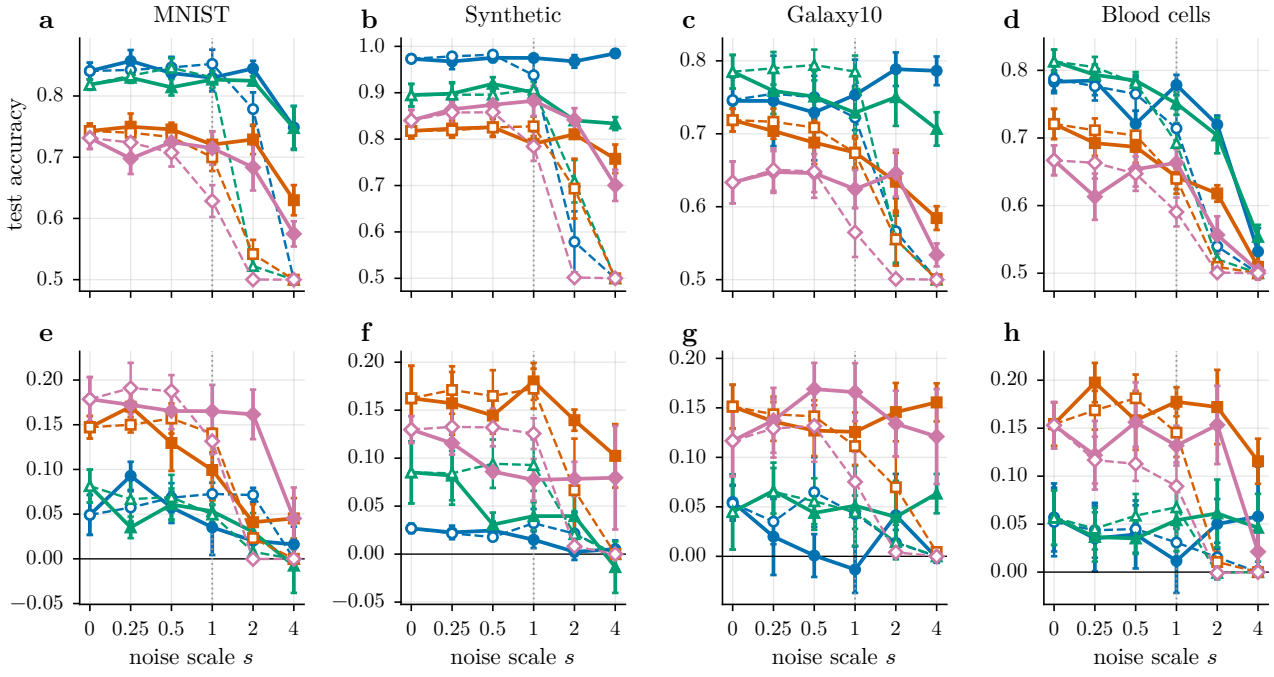
a
MNIST
b
Synthetic
c
Galaxy10
d
Blood cells
test accuracy
e
f
g
h
generalization gap
noise scale s
Equiv
Twirled
NonEquiv
NoSym
trained and tested under noise
trained without noise, tested under noise