

Production: PICKLE

Objective: Measurement of the firmness of pickle

Type of action: Cutting test

Test mode settings:

Speed	Test mode	Trigger	Target	Hold
3 mm/s	Distance (c)	0 gf	43 mm	0 sec

Accessory:

Kramer shear cell - 10 blades, Platform

Sample Preparation:

Remove the pickle from its container and weigh out into equal portions. It is important that enough is weighed out to approximately fill the Shear Cell by 50% of its capacity.

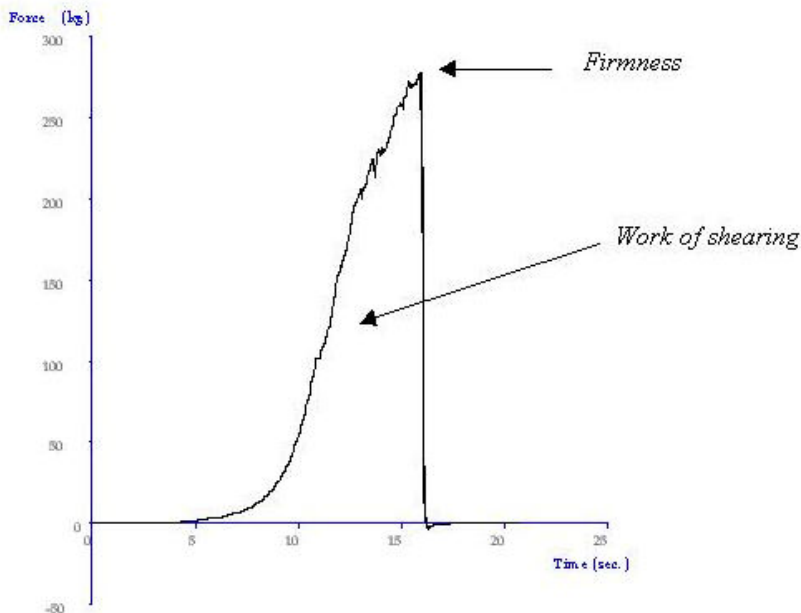
Test Set-Up:

The empty Shear Cell (Perspex front forward) is secured in the Heavy Duty Platform, which is loosely fixed onto the machine base. The blades are attached to the load cell carrier by means of the rapid locating adapter and lowered slowly into the sample cell and through the base slots. The Heavy Duty platform is then moved until clearance is visible between the blades and their respective slots. The Heavy Duty Platform can then be screwed into place.

Before carrying out the test using a 'zero' trigger one must calibrate the blades to acknowledge the bottom of the cell as a zero position. To do this, lower the blades, so that they close to the bottom of the cell. Click on **CALIBRATE HEIGHT**. Specify the distance that you want the blades to start from for each test - e.g. **45mm** is suggested. (Note: place a piece of thin flat card in the bottom of the cell to calibrate and then remove this before testing.)

The blades will move down and touch the card and then move up to the specified start distance. For the comparison of results it is crucial that the test always begins at the same distance from the bottom of the cell, this distance can be programmed into the **CONTROL PROBE** feature.

Prior to each test ensure that there is good clearance around the blades to avoid frictional effects, i.e. so that the blades are not touching the sides of the cell. The blades are then raised above the cell to allow for placement of the test sample. Running a spatula (or other) horizontally across the outside edges of the blades is recommended to ensure that the blades are hanging freely. Place the sample into the cell, distribute pieces evenly and run the test. In between tests clean the blades and the grooves of the cell to remove any remaining sample, as this will cause variable results.

Typical plots:

The above curve was produced from 300g of 'chunky' pickle tested at 20C.

Observations:

Once the blades have reached the sample, force is seen to increase at a steady rate. As the blades move down further onto the sample the force begins to increase rapidly as the sample begins to deform and rupture. After rupturing has occurred the subsequent increase in force is as a result of the force required to shear and extrude the sample through the slots in the base of the cell.

Data Analysis:

☒ Max Force

Results

Sample	Mean Maximum Force 'Firmness' (+/- S.D.) (kg)	Mean Area 'Work of Shearing' (+/- S.D.) (kg·s)
A	277.9 +/- 12.5	1195.1 +/- 43.8

Notes:

- The Kramer shear cell is a multi-bladed device. The sample to be sheared is often variable configuration or structure. The result is an average of the forces required to cut through the sample of variable geometry.
- If the sample is firmer or it is preferable to shear to a greater extent, a 500kg load cell would be recommended for a higher force range.
- When attempting to optimize test settings it is suggested that the first tests are performed on the hardest samples to anticipate the maximum testing range required and ensure that the force capacity allows testing of all future samples.