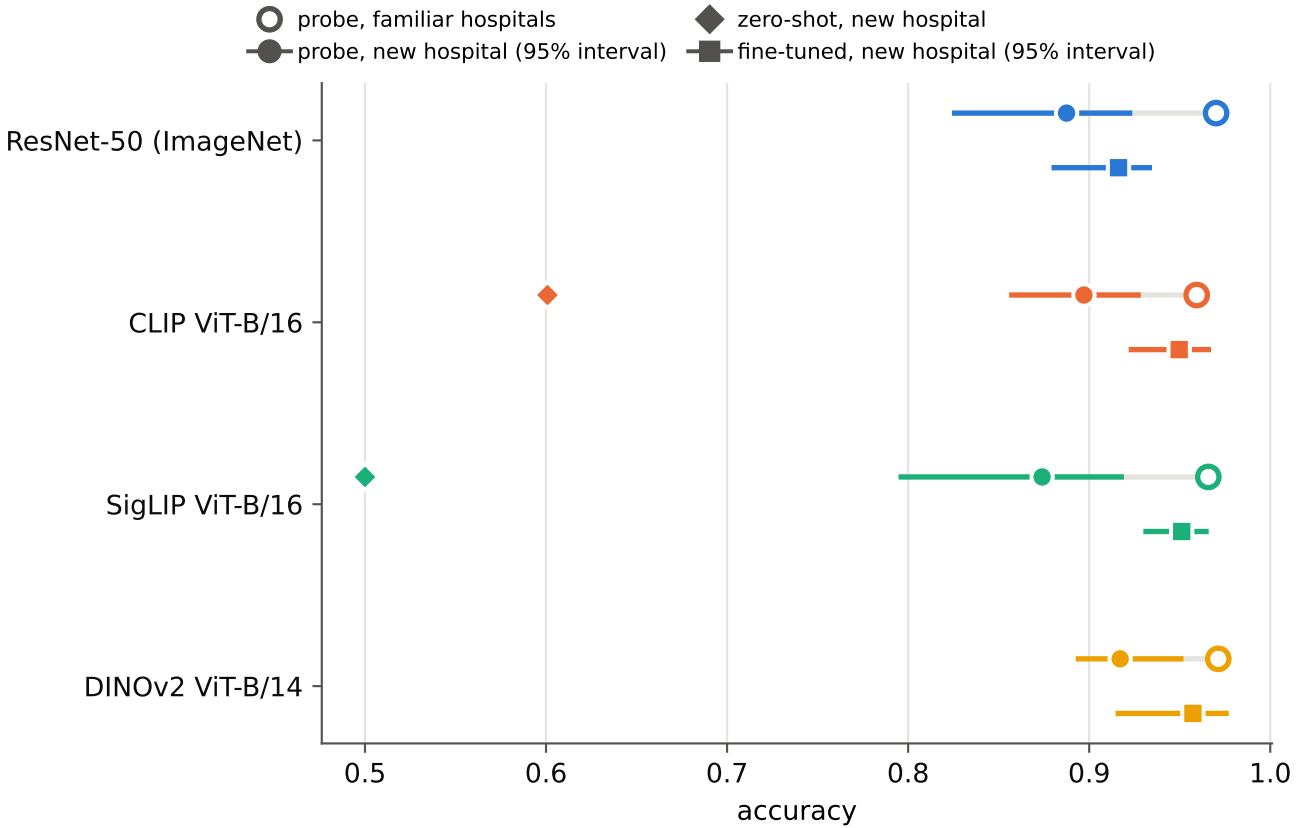
probe, familiar hospitals
zero-shot, new hospital
probe, new hospital (95% interval)
fine-tuned, new hospital (95% interval)
ResNet-50 (ImageNet)
CLIP ViT-B/16
SigLIP ViT-B/16
DINOv2 ViT-B/14
0.5
0.6
0.7
0.8
0.9
1.0
accuracy