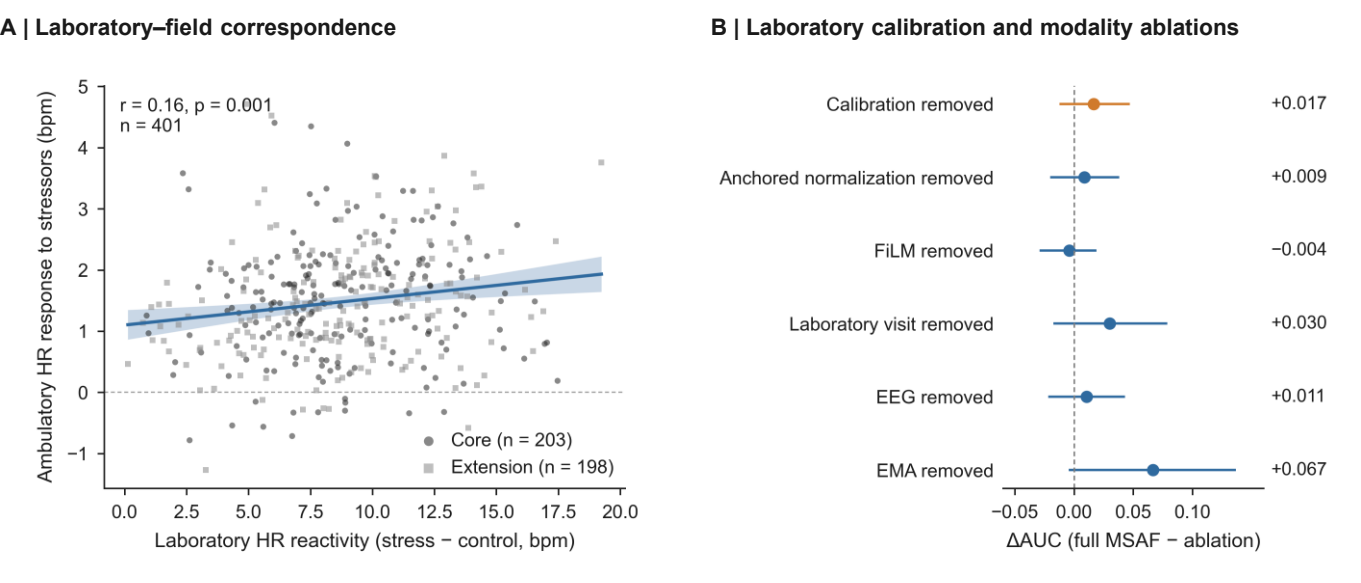

A | Laboratory–field correspondence
r = 0.16, p = 0.001
n = 401
Core (n = 203)
Extension (n = 198)
Ambulatory HR response to stressors (bpm)
Laboratory HR reactivity (stress − control, bpm)
5
4
3
2
1
0
−1
0.0
2.5
5.0
7.5
10.0
12.5
15.0
17.5
20.0
B | Laboratory calibration and modality ablations
Calibration removed
Anchored normalization removed
FiLM removed
Laboratory visit removed
EEG removed
EMA removed
+0.017
+0.009
−0.004
+0.030
+0.011
+0.067
−0.05
0.00
0.05
0.10
ΔAUC (full MSAF − ablation)