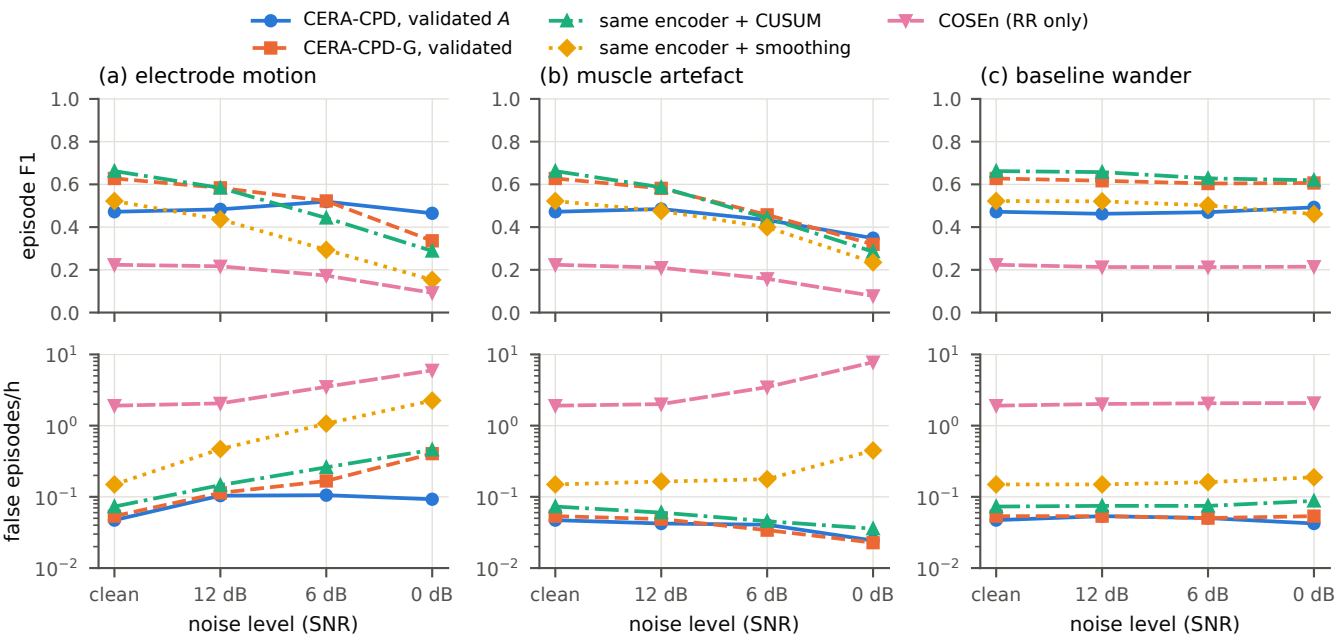
CERA-CPD, validated A
CERA-CPD-G, validated
same encoder + CUSUM
same encoder + smoothing
COSEn (RR only)
(a) electrode motion
(b) muscle artefact
(c) baseline wander
episode F1
false episodes/h
clean
12 dB
6 dB
0 dB
noise level (SNR)