

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
कोचर पैटर्न विच्छेदनकर्ता — विशिष्टि
(IS 7521 का पहला पुनरीक्षण)

Draft Indian Standard
Kocher Pattern Dissector — Specification
(First Revision of IS 7521)

ICS 11.040.30

Surgical Instruments Sectional Committee, MHD 01 Last date for comments: **30 September 2026**

FOREWORD

(Formal clauses will be added later)

This Indian Standard (First Revision) was first published in 1974 as ‘Specification for Dissector, Kocher’s Pattern’. This revision aligns the cross references to the latest standards, incorporates revised designations for steel and revised certification clause.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2 : 2022 ‘Rules for rounding off numerical values (second revision)’. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This Indian Standard covers dimensional and other requirements for Kocher's pattern dissector used in general surgery.


2 REFERENCES

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
IS 1070 : 2023	Reagent Grade Water Specification (<i>fourth revision</i>)
IS 6603 : 2024	Stainless Steel Semi-Finished Products, Bars, Wire Rods and Bright Bars - Specification (<i>second revision</i>)
IS 7531 : 1990	Surgical Instruments - Corrosion resistance of Stainless Steel Surgical Instruments - Methods of Tests (<i>first revision</i>)

3 SHAPE AND DIMENSIONS

Shape and dimensions shall be as shown in Fig. 1.

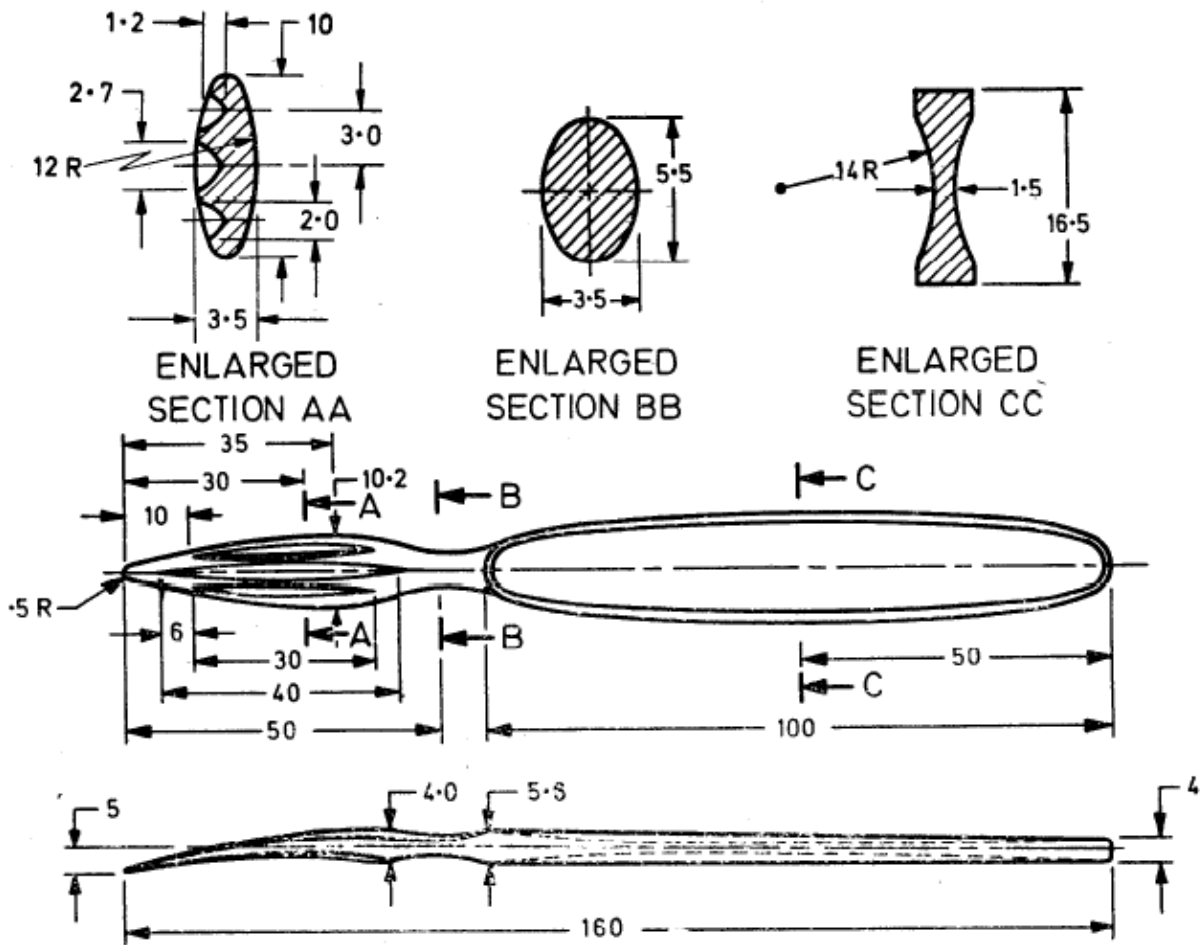

All dimensions in millimetres.

FIG. 1 KOCHER PATTERN DISSECTOR

4 MATERIAL

Stainless steel conforming to Designation X20Cr13 or X30Cr13 of IS 6603.

5 WORKMANSHIP AND FINISH

5.1 The dissector shall be free from burrs, pits, cracks, scales and other surface defects.

5.2 All edges including tip shall be even.

5.3 The dissector shall be polished bright and passivated.

6 HEAT TREATMENT

The dissector shall be hardened and tempered to give a hardness of 400 to 460 *HV*.

7 TESTS

7.1 Rigidity Test

Hold the dissector from the blade end in a suitable vice so that a length of 135 mm projects above the jaws. Apply a load of 170 N on the handle at a point 35 mm from its end. Attain the maximum load gradually and allow it to act for two minutes. On completion of the test the dissector shall not have acquired a permanent set.

7.2 Corrosion Resistance Test

The dissector shall satisfy the boiling and autoclaving test as mentioned in IS 7531.

7.2.1 Subject to agreement between the purchaser and the supplier, the dissector may be put to the following test:

7.2.1.1 Copper Sulphate Test

Scrub the sample with soap and warm water, rinse in shot water and then dip in 95 percent ethyl alcohol. Dry the sample. Immerse in copper sulphate solution at room temperature for 6 minutes and wash off with fresh water or swab with wet cotton wool. Composition of the solution shall be as follows:

Copper sulphate ($\text{CuSO}_4 \cdot 5\text{H}_2\text{O}$)	4.0 g
Sulphuric acid (H_2SO_4) (sp gr 1.84)	10.0 g
Reagent Water (<i>see</i> IS 1070)	90.0 ml

No red stains or spots on the dissector shall be allowed but dulling of the polished surface may be permitted.

8 MARKING

8.1 Mark with the following:

- a) Manufacturer's name, initials or his recognized trade-mark; and
- b) The words 'Stainless Steel'.

8.2 BIS Certification Marking

The product(s) confirming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

9 PACKING

Each dissector shall be wrapped in moisture-proof paper and put in a cardboard carton or shall be packed in a polyethylene bag. Dissectors may also be packed as agreed to between the purchaser and the supplier.