

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा

वॉटसन चेनी पैटर्न विच्छेदनकर्ता — विशिष्टि

(IS 8031 का पहला पुनरीक्षण)

Draft Indian Standard

Watson Cheyne Pattern Dissector — Specification

(First Revision of IS 8031)

ICS 11.040.30

Surgical Instruments Sectional Committee, MHD
01

Last date for comments: 30 September
2026

FOREWORD

(Formal clauses will be added later)

This Indian Standard (First Revision) was first published in 1976 as ‘Specification for Dissector, Watson Cheyne’s Pattern’. This revision aligns the cross references to the latest standards, incorporates revised designations for steel and revised certification clause.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2 : 2022 ‘Rules for rounding off numerical values (second revision)’. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

This Indian Standard covers dimensional and other requirements for Watson Cheyne's pattern dissector used in general surgery.

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
IS 6603 : 2024	Stainless Steel Semi-Finished Products, Bars, Wire Rods and Bright Bars - Specification (<i>second revision</i>)
IS 7531 : 1990	Surgical Instruments - Corrosion resistance of Stainless Steel Surgical Instruments - Methods of Tests (<i>first revision</i>)

3.1 Shape and dimensions shall be as shown in Fig. 1.

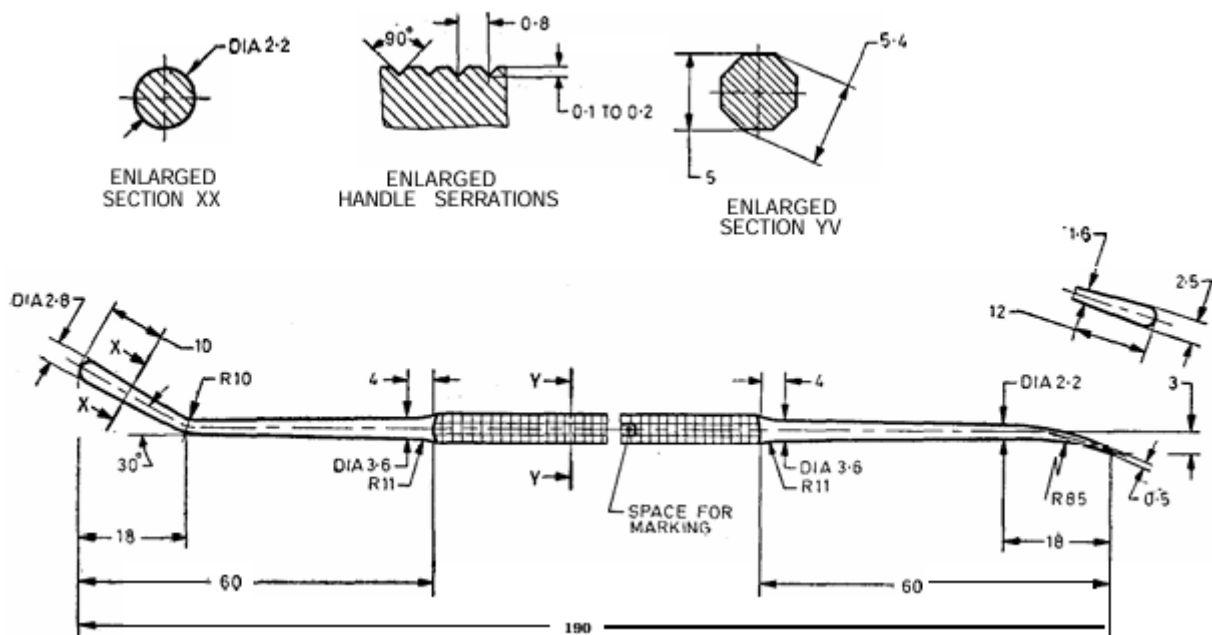


FIG. 1 WATSON CHEYNE PATTERN DISSECTOR

4 MATERIAL

Dissector shall be of stainless steel conforming to Designation 20Cr13 or 30Cr13 of IS 6603.

5 WORKMANSHIP AND FINISH

5.1 The ends of the dissector shall be sharp as shown in Fig 1.

5.2 The dissector shall be free from pits, cracks, burrs and other surface flaws.

5.3 The dissector shall be polished bright and passivated.

6 HEAT TREATMENT

The dissector shall be hardened and tempered to give a hardness of 380 to 430 *HV*.

7 TESTS

7.1 Flexibility Test

7.1.1 Hold the dissector in a vice at the middle so that its flat end points upwards and 86 mm of the shaft protrudes above the vice. Apply a force at the tip of the flat end, so as to deflect it in a plane at right angles to the long axis of the jaw of the vice by 7 mm as measured at the upper extremity of the flat end. On release of the force, no permanent set shall be observed.

7.1.2 Repeat the test with the dissector fixed at the middle of the shaft and the round end pointing upwards. Apply the force to the shaft at a point 86 mm above the upper surface of the vice in a plane at right angles to the long axis of the jaw of the vice. Deflect the shaft by 7 mm as measured at the level of the point where the force is applied. On release of the force, no permanent set shall be observed.

7.2 Corrosion Resistance Test

Test the dissector in accordance with IS 7531.

8 MARKING

8.1 Each dissector shall be legibly and indelibly marked with the manufacturer's initials or his recognized trade-mark.

8.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

9 PACKING

As agreed to between the purchaser and the supplier.