

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
गुर्दाकार बर्तन - विशिष्टि
[IS 3992 का दूसरा पुनरीक्षण]

Draft Indian Standard
Kidney Shaped Tray — Specification
[Second Revision of IS 3992]

ICS 11.040.01

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1967 and subsequently revised in 1982. The second revision is brought out to align it with the latest material grade, addition of tolerance in the figure, removal of enamelled iron tray and to bring the standard to the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 ‘Rules for rounding off numerical values (*second revision*)’. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies the requirements of stainless steel kidney trays.

2 REFERENCES

The standards given below contain provisions, which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
IS 513 (Part 2): 2016	Cold reduced carbon steel sheet and strip: Part 2 high tensile and multi - Phase steel (<i>sixth revision</i>)
IS 2717: 2025	Vitreous Enamelware and Ceramic-Metal Systems - Glossary (<i>second revision</i>)
IS 3972 (Part 2/Sec 3): 2020 ISO 28706-2: 2017	Methods of Test for Vitreous Enamelware Part 2 Test Methods Section 3 Resistance to boiling acids, boiling liquids, alkaline liquids and their vapours (<i>second revision</i>)
IS 5522: 2014	Stainless steel sheets and strips for utensils - Specification (<i>third revision</i>)

3 TERMINOLOGY

The definitions which are used in this standard shall be as per IS 2717.

4 SHAPE AND DIMENSIONS

4.1 Shape

The shape of kidney trays shall conform to Fig. 1. The contour shall be in such a way that the trays of the same size when stacked together shall not become jammed. The contour of the sides shall bulge outside as shown in Fig. 1. The base of the kidney tray shall be flat.

4.1.1 The kidney trays shall have rim as shown in Fig. 1.

4.2 Dimensions


The dimensions and tolerance of kidney shaped trays shall be as given below:

<i>Dimensions (mm)</i>	<i>Tolerance (mm)</i>
Up to 50	±1
51 to 100	±2
101 to 200	±3
201 and above	±5

Table 1 DIMENSIONS OF KIDNEY TRAYS
All dimensions in millimetres

Length	Width	Height	Radius of Curvature			Minimum Thickness of Material
A	B	C	R1	R2	R3	Stainless Steel
(1)	(2)	(3)	(4)	(5)	(6)	(7)
150	70	30	75	90	45	0.45
200	90	40	100	120	60	
250	100	50	125	150	75	
250	150	40	170	150	125	
300	130	60	150	180	90	

4.3 A deviation of maximum 15 percent shall be permitted for negative tolerance on sheet thickness and the reduction in the drawing due to the forming process.

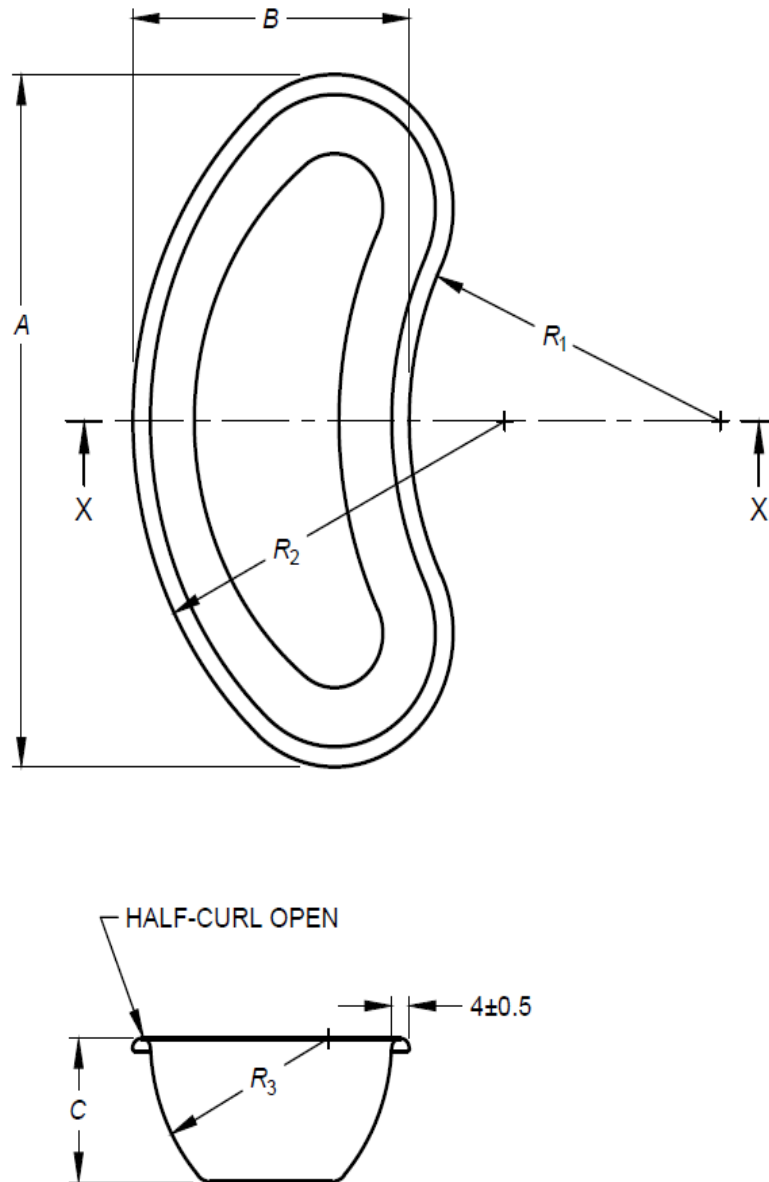

SECTION X-X

Fig. 1 KIDNEY SHAPED TRAY

5 MATERIAL REQUIREMENTS

5.1 Stainless Steel

The stainless steel material shall conform to Designation X07Cr18Ni9 of IS 5522.

6 WORKMANSHIP AND FINISH

6.1 The kidney shaped trays shall be constructed in such a way that these shall not rock when placed on a level surface.

6.2 Stainless Steel Trays

The trays shall be polished bright. These trays are free from sharp or open edges, distortion, dents, wrinkles, wavy surface, burrs, scratches and pitting.

7 MARKING

7.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the following:

- a) Identification of the manufacturer;
- b) Size of the tray.

7.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

8 PACKAGING

The kidney shaped tray shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one tray and may be marked with the name of the item, and identification of the source of manufacture and batch number and any other marking if so desired.