

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
बिस्तर के ऊपर की मेज - विशिष्टि
[IS 4494 का पहला पुनरीक्षण]

Draft Indian Standard
Overbed Tables - Specification
[First Revision of IS 4494]

ICS 11.140

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1968. The first revision of this standard has been brought out to align it with recent developments in the material requirements, removal of carton material, updation of marking and packaging requirements and to bring the standard in line with the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 'Rules for rounding off numerical values (*second revision*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies the requirements of fixed height overbed tables used in hospitals and other similar institutions.

2 REFERENCES

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
IS 4032: 1985	Method of Chemical Analysis of Hydraulic Cement (<i>first revision</i>)
MHD 12 (33411) WC (Under Development)	Hospital Furniture - General Requirements (<i>first revision</i>)
IS 17523: 2021	Castors and Wheels - Requirements for Castors for Furniture
IS 1868: 1996	Anodic coatings on aluminium and its alloys - Specification (<i>third revision</i>)

3 MATERIAL REQUIREMENTS

3.1 Framework

The material used for the framework shall be as per **3.1** of IS 4033.

3.2 Top

The top of the overbed table shall be made of 1 mm mild steel sheet layered by stainless steel sheet of minimum 0.5 mm thickness or aluminium sheet of 1 mm thickness having 10-micron anodic coating as per **Grade AC 10** of IS 1868.

4 SHAPE AND DIMENSIONS

4.1 The shape and dimensions of overbed tables shall be as per Fig. 1 to Fig. 3.

4.2 The tube used for the framework shall have thickness of 2.35 mm and outside diameter shall be greater than 26.9 mm. The tie bars for the tube shall have thickness of 2 mm and outside diameter greater than 213 mm.

4.3 The metal sheets used for the top shall have the following thickness:

<i>Material</i>	<i>Thickness</i>
	mm
Mild steel	1.00
Aluminium	1.25
Stainless steel	0.5

5 TYPES


5.1 The overbed tables shall have two types:

5.1.1 Type 1

The overbed table with top mounted on tubular metal framework which have legs over the bed or over the ground as desired by the purchaser as per Fig. 1 and Fig. 2.


5.1.2 Type 2

The overbed table with top mounted on a tubular metal framework which has legs fitted with castors as per Fig. 3.

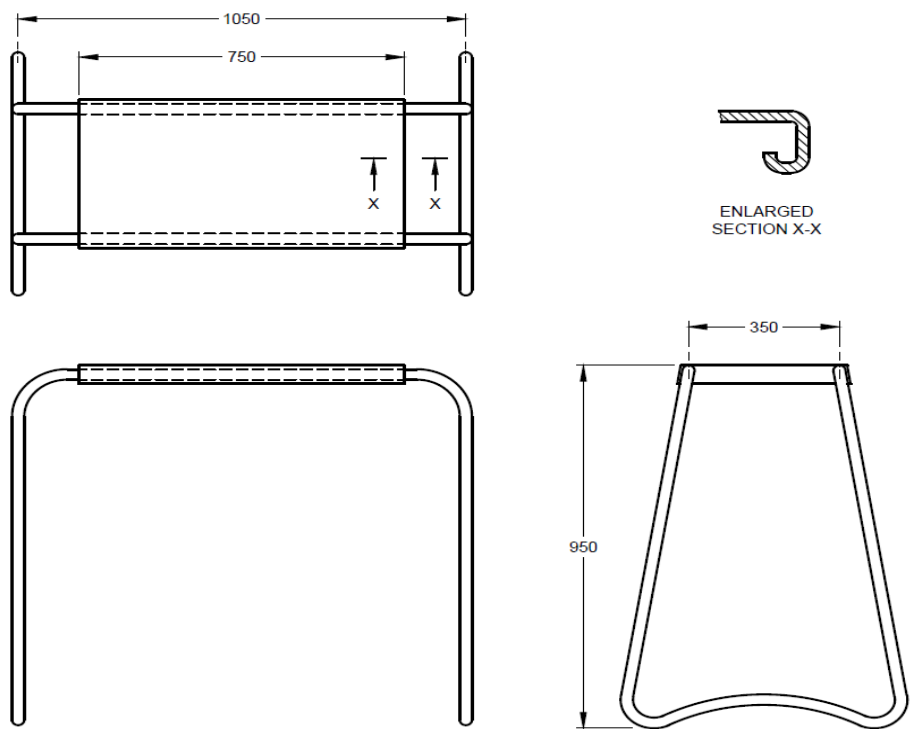


Tolerance on all dimensions ± 5 mm
All dimensions in millimetres

Fig. 1 OVERBED TABLE

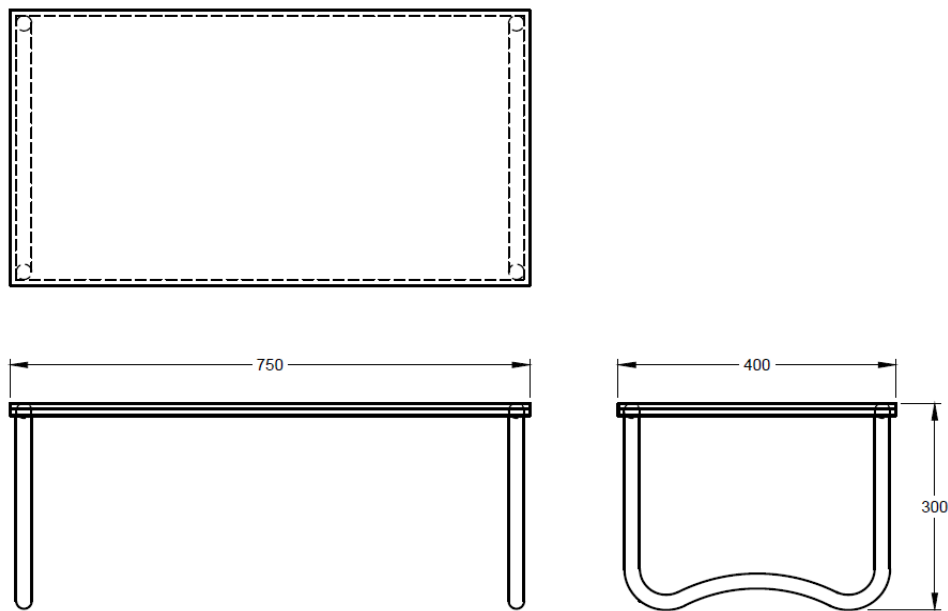

Tolerance on all dimensions ± 5 mm
All dimensions in millimetres

Fig. 2 OVERBED TABLE

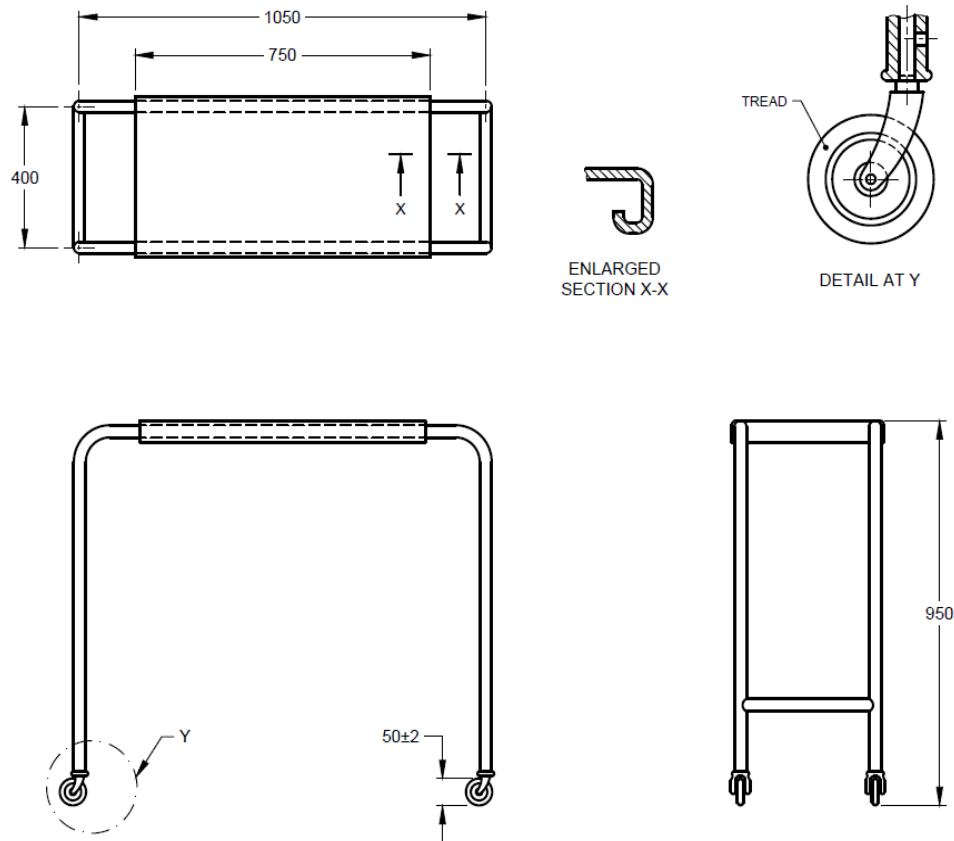

Tolerance on all dimensions ± 5 mm except where specified
All dimensions in millimetres.

Fig. 3 OVERBED TABLE

6 CONSTRUCTION REQUIREMENTS

6.1 The overbed tables shall have a framework of continuous length mild steel tubes as shown in the figures. The tubes shall be bent to act as tie bars (see type 1 overbed tables). The type 2 overbed table shall have two pairs of legs of the table connected by tie rods as shown in Fig. 3. The sheet metal top shall be attached to the longitudinal members of the framework by rolling over and soldering or securely fastened to the framework. The mild steel used for the top shall be superimposed with a laminated sheet. The rest of the details shall be as per 5.1 of IS 4033.

6.2 Castors

The castor for type 2 overbed table provided with four castors which shall conform to IS 17523. The additional requirements shall be as per 5.2 of IS 4033.

7 TESTING REQUIREMENTS

The testing for an overbed table shall be as per 6 of IS 4033, and the performance shall be determined by putting additional load on the overbed table (this test is only applicable for Type 2 tables).

8 WORKMANSHIP AND FINISH

The finish for the overbed table shall be in accordance with 7 of IS 4033.

9 MARKING

9.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the Identification mark of the manufacturer.

9.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

10 PACKAGING

The overbed table shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one unit and may be marked with the name of the item, and identification of the source of manufacture and batch number and any other marking if so desired.