

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
मरहम-पट्टी के सामान हेतु पहियेदार मेज - विशिष्टि
[IS 4769 का पहला पुनरीक्षण]

Draft Indian Standard
Dressing Trolley - Specification
[First Revision of IS 4769]

ICS 11.140

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1968. The first revision of this standard has been brought out to align it with recent developments in the material requirements, updation of washbowl and instrument tray requirements and to bring the standard in line with the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 'Rules for rounding off numerical values (*second revision*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies the requirements of dressing trolleys used in hospitals and other similar institutions.

2 REFERENCES

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
MHD 12 (33411) WC (Under Development)	Hospital Furniture - General Requirements (<i>first revision</i>)
MHD 12 (28623) WC (Under Development)	Instrument Tray — Specification (<i>third revision</i>)
MHD 12 (28631) WC (Under Development)	Hand Wash Basin and Stand - Specification (<i>first revision</i>)
IS 1068: 2025 ISO 1456: 2009	Metallic and other inorganic coatings - Electrodeposited coatings of nickel, nickel plus chromium, copper plus nickel and of copper plus nickel plus chromium (<i>fourth revision</i>)
IS 5522: 2014	Stainless steel sheets and strips for utensils - Specification (<i>third revision</i>)
IS 17523: 2021	Castors and Wheels - Requirements for Castors for Furniture

3 TERMINOLOGY

3.1 Dressing Trolley - The dressing trolleys used for the purpose of dressing at the bedside in the wards or dressing rooms.

4 MATERIAL

4.1 Framework

The material used for the framework shall be as per **3.1** of IS 4033.

4.2 Shelves

The shelves shall be made from polished glass having a minimum thickness of 6 mm. The shelves may also be made from stainless steel sheet conforming to IS 5522 with minimum thickness of 0.8 mm.

4.3 Pivot Bar, Rings and Disc

The pivot bar, rings and disc shall be made from mild steel which is either of cold-rolled or hot-rolled quality.


4.4 Castors

The castor which is used for trolley shall conform to the requirements as per IS 17523.

5 DIMENSIONS

5.1 The dimensions of the trolley shall be as given in Fig. 1.

5.2 The outside diameter and thickness of the tubes used for framework shall be as per below:

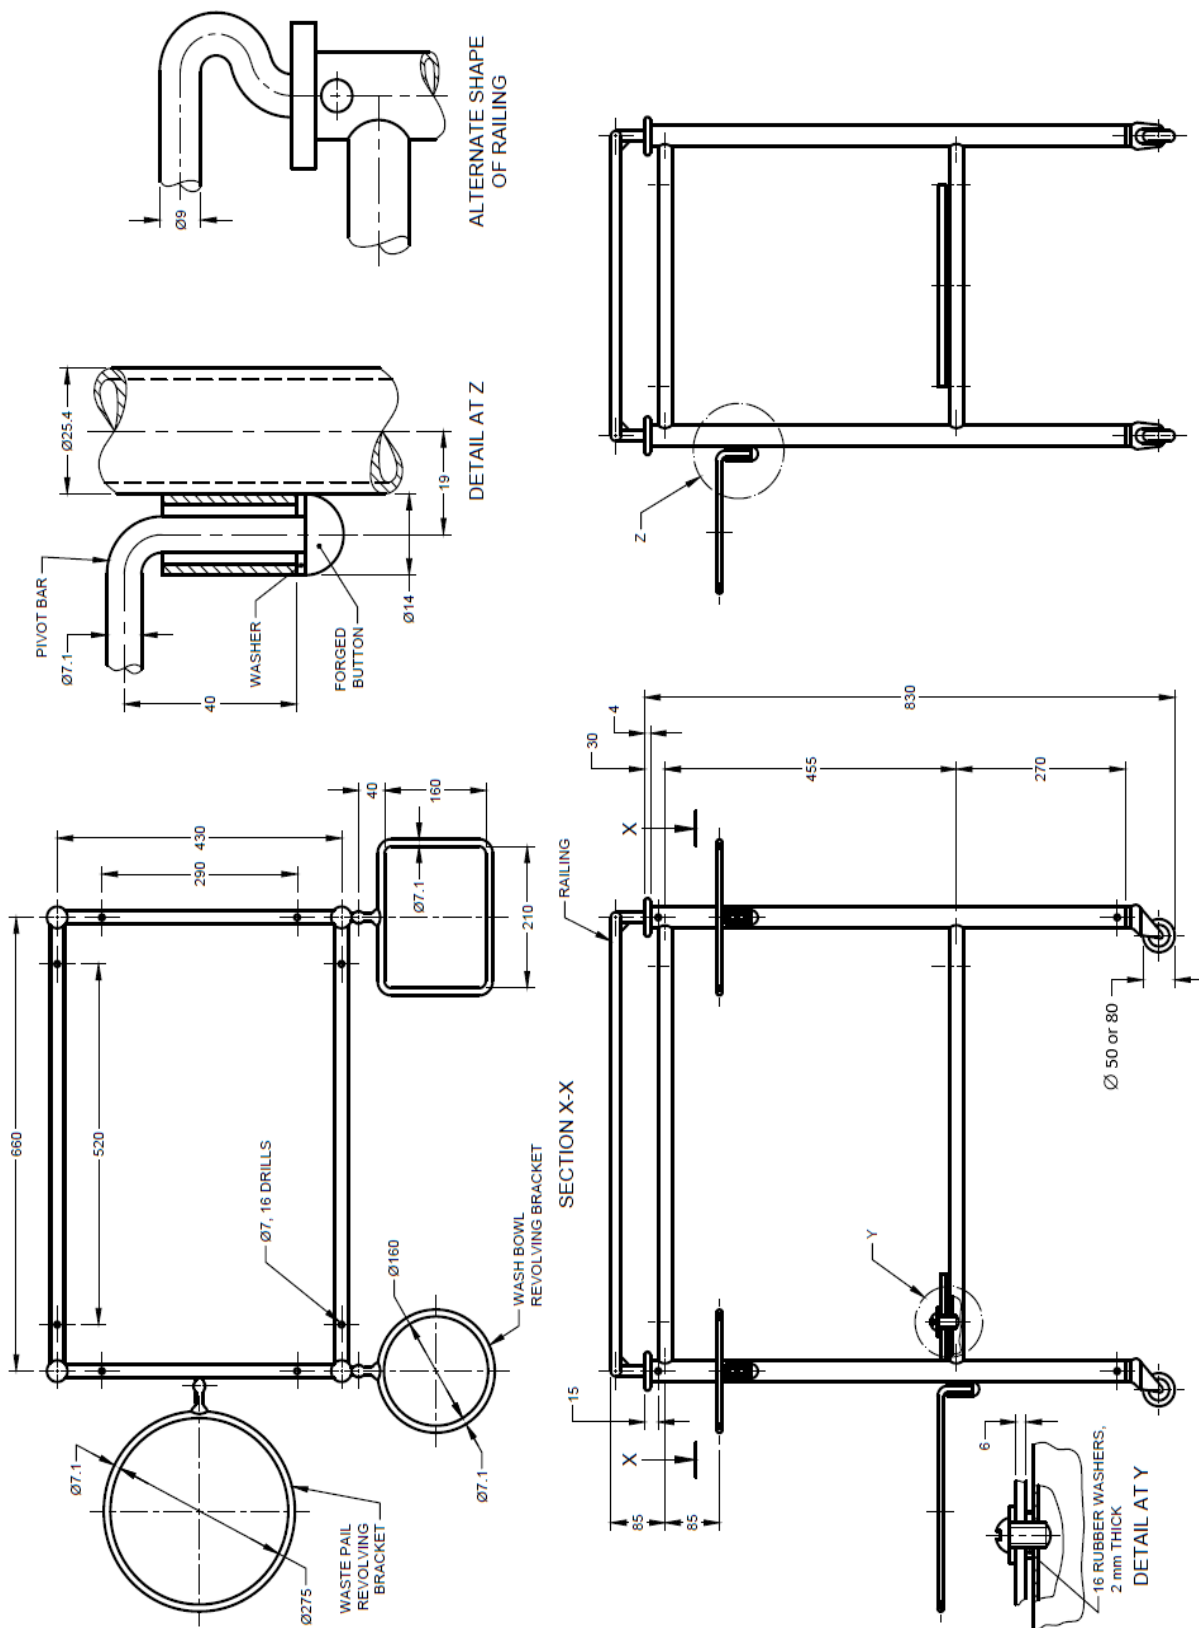

Tolerance on all dimensions ± 5 mm

All dimensions in millimetres

Fig. 1 DRESSING TROLLEY

<i>Member</i>	<i>Thickness of Tube</i>	<i>Outside Diameter of Tube</i>
	mm	mm
Vertical	1.20	25.40
Horizontal	1.20	19.05

6 CONSTRUCTION REQUIREMENTS

6.1 Framework

The dressing trolley shall have a framework of single continuous length mild steel tubes as shown in Fig. 1. The frame has four upright members connected together by a pair of longitudinal and a pair of transverse tie rods. The two longitudinal and two transverse tie rods shall be connected to the four upright members in such a way that they form a supporting frame for shelves which are suitable for receiving round edged plate glass shelves. The top shelf shall be provided with a chromium-plated railing on three sides.

6.2 Wash Bowl

The wash bowl placed on the revolving bracket shall be as per IS 4267.

6.3 Instrument Tray

The instrument tray placed on the revolving bracket shall be as per IS 3993.

6.4 Castors

The trolley provided with four castors shall have diameter 50 mm made from antistatic rubber tread conform to IS 17523. The additional requirements shall be as per 5.2 of IS 4033.

6.5 The left side shall have an attachment to provide a waste pail as shown in Fig. 1.

7 TESTING REQUIREMENTS

7.1 Adhesion Test

The adhesion test required for the dressing trolley shall conform to 6.1.1 of IS 4033.

7.2 Performance Test

The performance test for the dressing trolley shall be as per 6.1.2 of IS 4033 which is tested by putting additional load.

7.2.1 The performance test shall be carried out and it is noted that the shelves shall not get displaced or make rattling noise.

8 WORKMANSHIP AND FINISH

8.1 The finish for the instrument trolley shall be in accordance with 7 of IS 4033. The shelves shall be free from sharp edges and corners.

8.2 The railing shall be chromium-plated over nickel and the plating shall conform to **Service Condition 2** of IS 1068.

9 MARKING

9.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the Identification mark of the manufacturer.

9.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

10 PACKAGING

The dressing table shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one unit and may be marked with the name of the

item, and identification of the source of manufacture and batch number and any other marking if so desired.