

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
परीक्षण के लिए मेज - विशिष्टि
[IS 4787 का पहला पुनरीक्षण]

Draft Indian Standard
Examination Table - Specification
[First Revision of IS 4787]

ICS 11.140

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1968. The first revision of this standard has been brought out to align it with recent developments in the material requirements, addition of tolerance to all dimensions and to bring the standard in line with the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 'Rules for rounding off numerical values (*second revision*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies the requirements of examination tables used in hospitals and other similar institutions.

2 REFERENCES

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
MHD 12 (33411) WC (Under Development)	Hospital Furniture - General Requirements (<i>first revision</i>)
IS 2835: 1987	Specification for flat transparent sheet glass (<i>third revision</i>)
IS 5522: 2014	Stainless steel sheets and strips for utensils - Specification (<i>third revision</i>)
IS 17523: 2021	Castors and Wheels - Requirements for Castors for Furniture

3 TERMINOLOGY

3.1 Examination Table - The table used for examination of patients in the consulting rooms, clinics and side-rooms of hospital wards.

4 MATERIAL REQUIREMENTS

4.1 Framework

The material used for the framework shall be as per **3.1** of IS 4033.

4.2 Top

The minimum thickness of the metal sheet used for top shall be 1.2 mm in case of mild steel or 1 mm in case of stainless steel. If the top is superimposed by stainless steel then the minimum thickness of stainless steel shall be 0.5 mm over a mild steel sheet of 0.8 mm thickness.

4.3 Rods, Channels and Strips

The rods, channels and strips shall be made up of mild steel which is either cold rolled or hot rolled quality.

5 SHAPE AND DIMENSIONS


5.1 The shape and dimensions of the examination table shall be as per Fig. 1.

5.2 The thickness of tubes used along with corresponding outside diameters for different parts shall be as given below:

<i>Part</i>	<i>Outside Diameter of Tube mm</i>	<i>Thickness of Tube mm</i>
Vertical members	31.75	1.02
Horizontal members	25.40	

5.3 The mild steel sheet used for the top and headrest shall have a minimum thickness of 1.22 mm.

5.4 The details given at section 'XX' and 'CC' in Fig. 1 shall be optional.

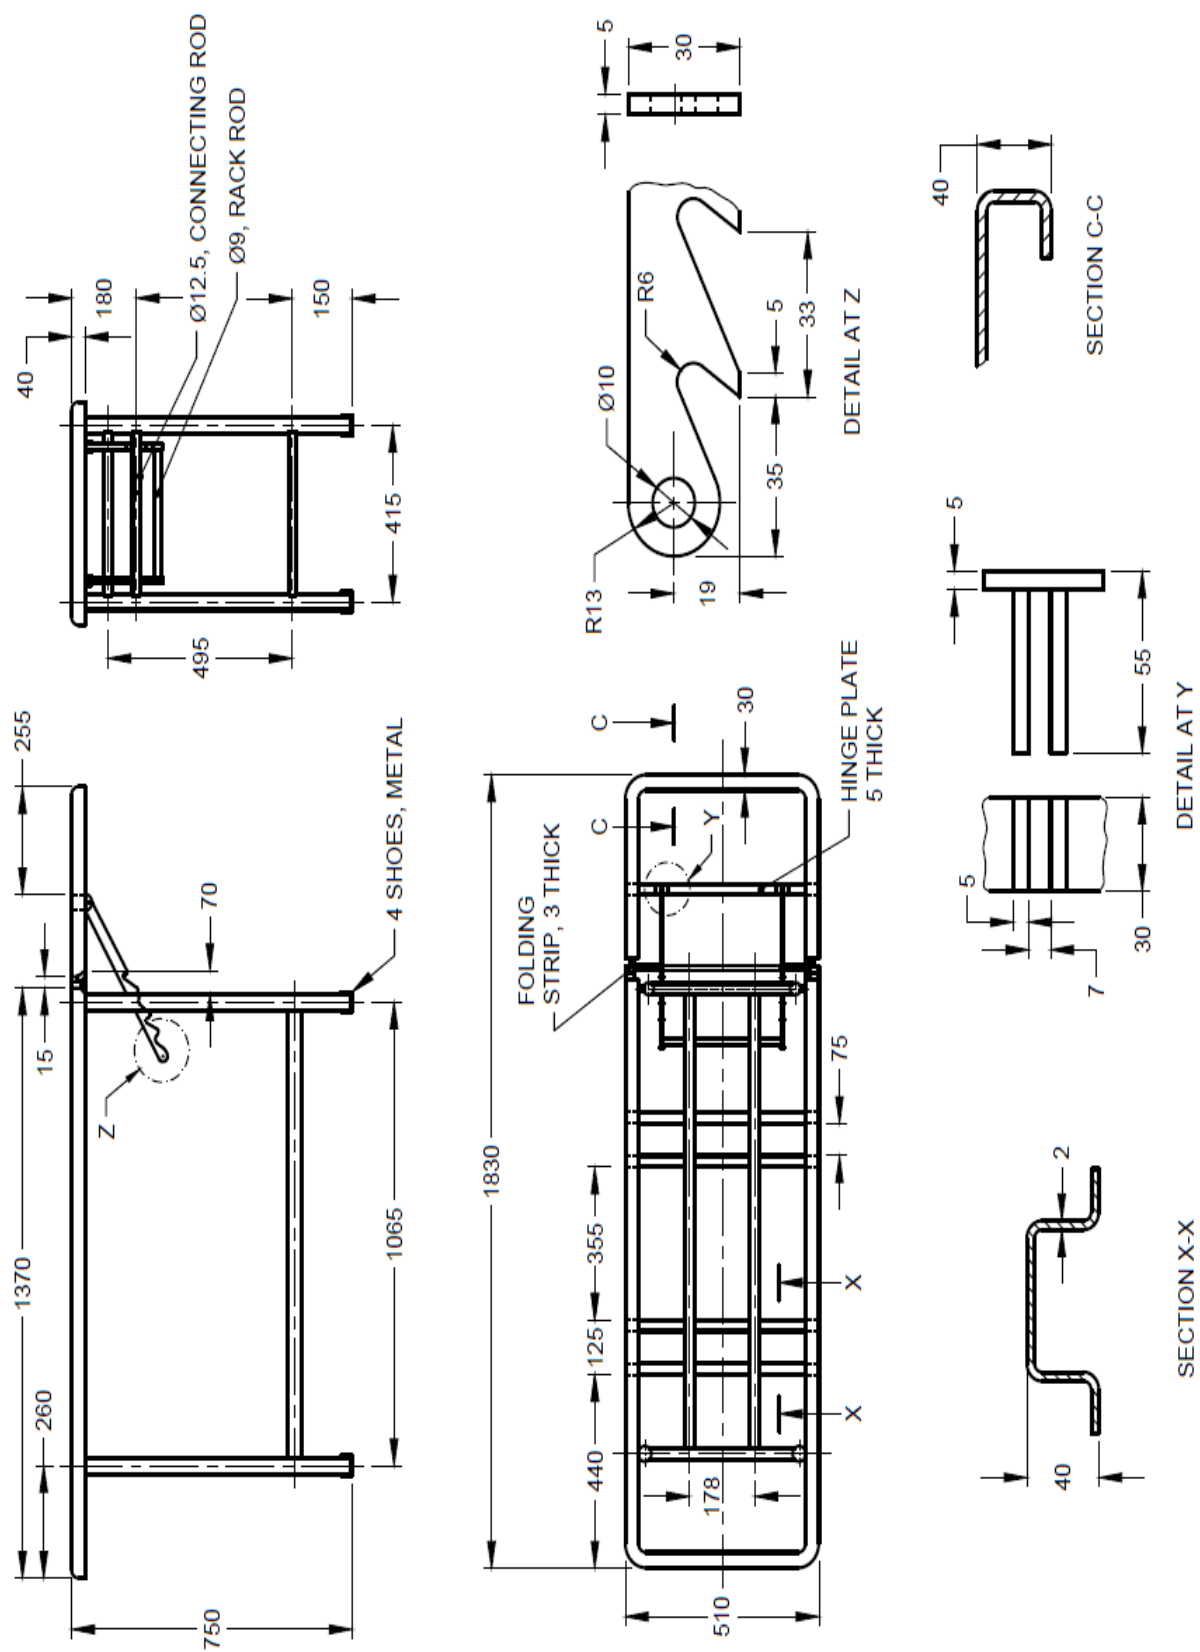

Tolerance on all dimensions ± 5 mm
All dimensions in millimetres
Fig. 1 EXAMINATION TABLE

6 CONSTRUCTION REQUIREMENTS

6.1 Framework

The examination table shall have a framework of single continuous lengths of mild steel tubes as shown in Fig. 1. The four upright members shall be connected together by longitudinal and transverse tie rods. The other end shall support a formed sheet metal top at the end of the floor. The sheet metal top shall be mounted at which the ends at uprights are flattened and thereafter welded to the top. Any other arrangement of fixing the sheet metal top to the framework shall be agreed to by the purchaser and the manufacturer in any case the top obtained shall be sturdy in construction. The headrest shall have the same construction as the top and it shall be adjustable on a rack for obtaining various positions. The floor ends of the upright members or legs shall be fitted with metal shoes. The rest of the details shall be according to 5 of IS 4033.

7 TESTING REQUIREMENTS

7.1 Adhesion Test

The adhesion test required for the examination table shall conform to 6.1.1 of IS 4033.

7.2 Performance Test

The performance test for the headrest of the examination table shall be tested with a load of 25 kgf spread over the entire width of head rest. The examination table shall be checked for excessive sideways play and stability for headrest.

8 WORKMANSHIP AND FINISH

The finish for the examination table shall be in accordance with 7 of IS 4033.

9 MARKING

9.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the Identification mark of the manufacturer.

9.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

10 PACKAGING

The examination table shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one unit and may be marked with the name of the item, and identification of the source of manufacture and batch number and any other marking if so desired.