

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा

उपकरणों के लिए समतल एवं घुमावदार पहियेदार मेज - विशिष्टि
[IS 5631 का पहला पुनरीक्षण]

Draft Indian Standard

Plain and Curved Shaped Instrument Trolley - Specification
[First Revision of IS 5631]

ICS 11.140

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1968. The first revision of this standard has been brought out to align it with recent developments in the material requirements, addition of workmanship and finish and to bring the standard in line with the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 'Rules for rounding off numerical values (*second revision*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies dimensional and construction requirements for plain and curved instrument trolleys.

2 REFERENCES

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
MHD 12 (33411) WC (Under Development)	Hospital Furniture - General Requirements (<i>first revision</i>)
IS 2835: 1987	Specification for flat transparent sheet glass (<i>third revision</i>)
IS 5522: 2014	Stainless steel sheets and strips for utensils - Specification (<i>third revision</i>)
IS 17523: 2021	Castors and Wheels - Requirements for Castors for Furniture

3 MATERIAL REQUIREMENTS

3.1 Framework

The material used for the framework shall be as per **3.1** of IS 4033.

3.2 Shelves


The shelves shall be made up of transparent sheet glass with 55 ± 0.3 mm thickness conforming to IS 2835 or stainless steel sheet of minimum thickness 8 mm conforming to IS 5522.

3.3 Disc

The disc used shall be made up of mild steel or aluminium.


4 SHAPE AND DIMENSIONS

The shape and dimensions of the instrument trolley shall be as per Fig. 1 and Fig. 2.

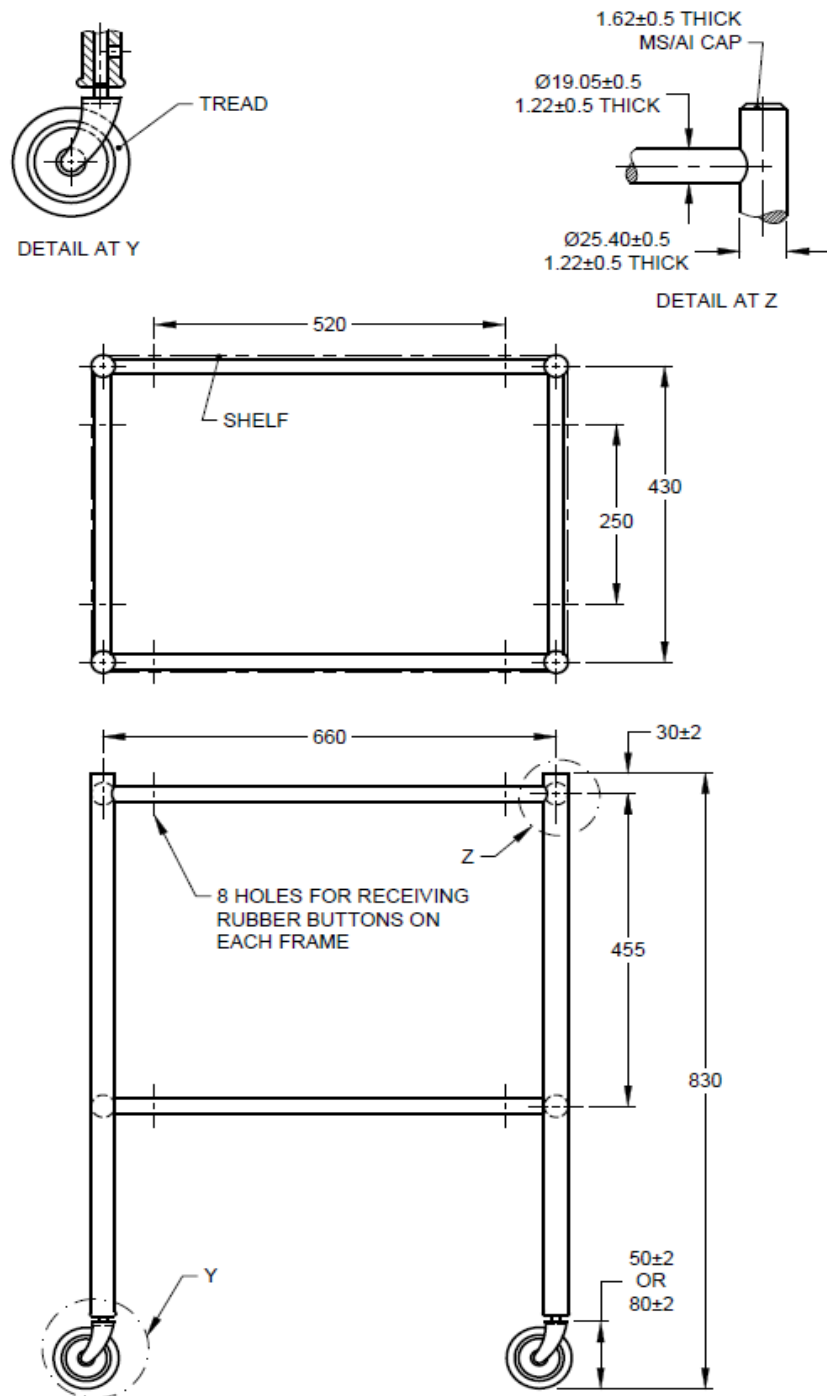

Tolerance on all dimensions ± 5 mm except where specified
All dimensions in millimetres

Fig. 1 PLAIN INSTRUMENT TROLLEY

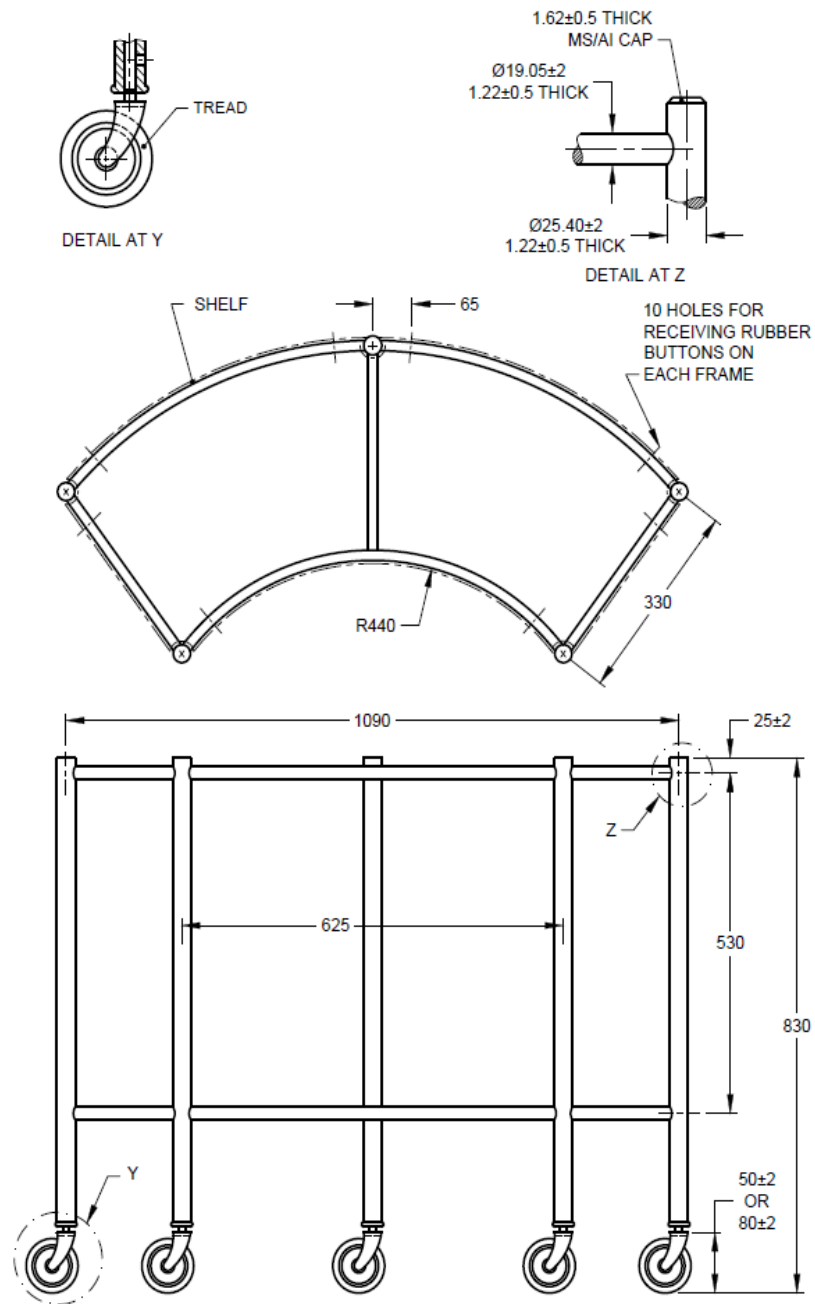

Tolerance on all dimensions ±5 mm except where specified
All dimensions in millimetres

Fig. 2 CURVED INSTRUMENT TROLLEY

5 CONSTRUCTION REQUIREMENTS

5.1 Framework

The framework that is used for the trolley shall be made with continuous mild steel tubes welded together as shown in Fig. 1 and Fig. 2. The upright members shall be connected together by another set of tubes as shown in the respective figures. These tubes shall be connected to the upright members in such a way to form supporting frames for two shelves, made of glass or stainless steel with shaped corners. The glass shelves are used to avoid rattling with suitable size rubber studs or buttons and the glass shelves pressed on them over the supporting frames. The curved instrument trolley shall have the shelves consisting of two equal segments. The upper ends of the upright members shall be sealed with mild steel or aluminium caps. The additional requirements for the trolley shall be as per 5.1 of IS 4033.

5.2 Castors

The trolley shall be provided with castors of 50 or 80 mm in diameter and antistatic rubber tread conforming to IS 17523.

NOTE — When antistatic rubber tread is not available the construction of the trolley shall otherwise ensure transmission of static charge to the earth.

6 TESTING REQUIREMENTS

6.1 Adhesion Test

The adhesion test required for the instrument trolley shall conform to 6.1.1 of IS 4033.

6.2 Performance Test

The performance test for the instrument trolley shall be as per 6.1.2 of IS 4033 which is tested by putting additional load.

6.2.1 The performance test shall be carried out and it is noted that the shelves shall not get displaced or make rattling noise.

7 WORKMANSHIP AND FINISH

The finish for the instrument trolley shall be in accordance with 7 of IS 4033. The shelves shall be free from sharp edges and corners.

8 MARKING

8.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the Identification mark of the manufacturer.

8.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act*, 2016 and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

9 PACKAGING

The instrument trolley shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one unit and may be marked with the name of the item, and identification of the source of manufacture and batch number and any other marking if so desired.