

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
सामान्य शल्य चिकित्सा के लिए मेज - विशिष्टि
[IS 6328 का पहला पुनरीक्षण]

Draft Indian Standard

General Purpose Non-Hydraulic Operation Table - Specification
[First Revision of IS 6328]

ICS 11.140

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1971. The first revision of this standard has been brought out to align it with recent developments in the material requirements, removal of wooden material for handle and to bring the standard in line with the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 'Rules for rounding off numerical values (*second revision*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies the construction and performance requirements of a manually controlled general-purpose operation table.

2 REFERENCES

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
MHD 12 (33411) WC (Under Development)	Hospital Furniture - General Requirements (<i>first revision</i>)
IS 6911: 2026	Stainless Steel Plate, Sheet and Strip - Specification (<i>third revision</i>)
IS 1068: 2025 ISO 1456: 2009	Metallic and other inorganic coatings - Electrodeposited coatings of nickel, nickel plus chromium, copper plus nickel and of copper plus nickel plus chromium (<i>fourth revision</i>)

3 TERMINOLOGY

3.1 General Purpose Operation Table - A surgical operation table capable of providing essential positions for various surgical procedures.

4 MATERIAL REQUIREMENTS

4.1 Framework

The material used for the framework shall be as per **3.1** of IS 4033.

4.2 Sheets, Rods and Flats

The components shall be made up of mild steel which is either cold rolled or hot rolled quality.


4.3 The additional components like the gearing system shall be made from materials that resist wear during normal manipulation.

4.4 The handles provided shall be made from ebonite or plastics which can stand the action of mild acids.

4.5 The stainless-steel components used shall conform to designation X07Cr17Ni12Mo2 in accordance with IS 6911.

5 SHAPE AND DIMENSIONS

The typical shape and dimensions of the operation table shall be as per Fig. 1.

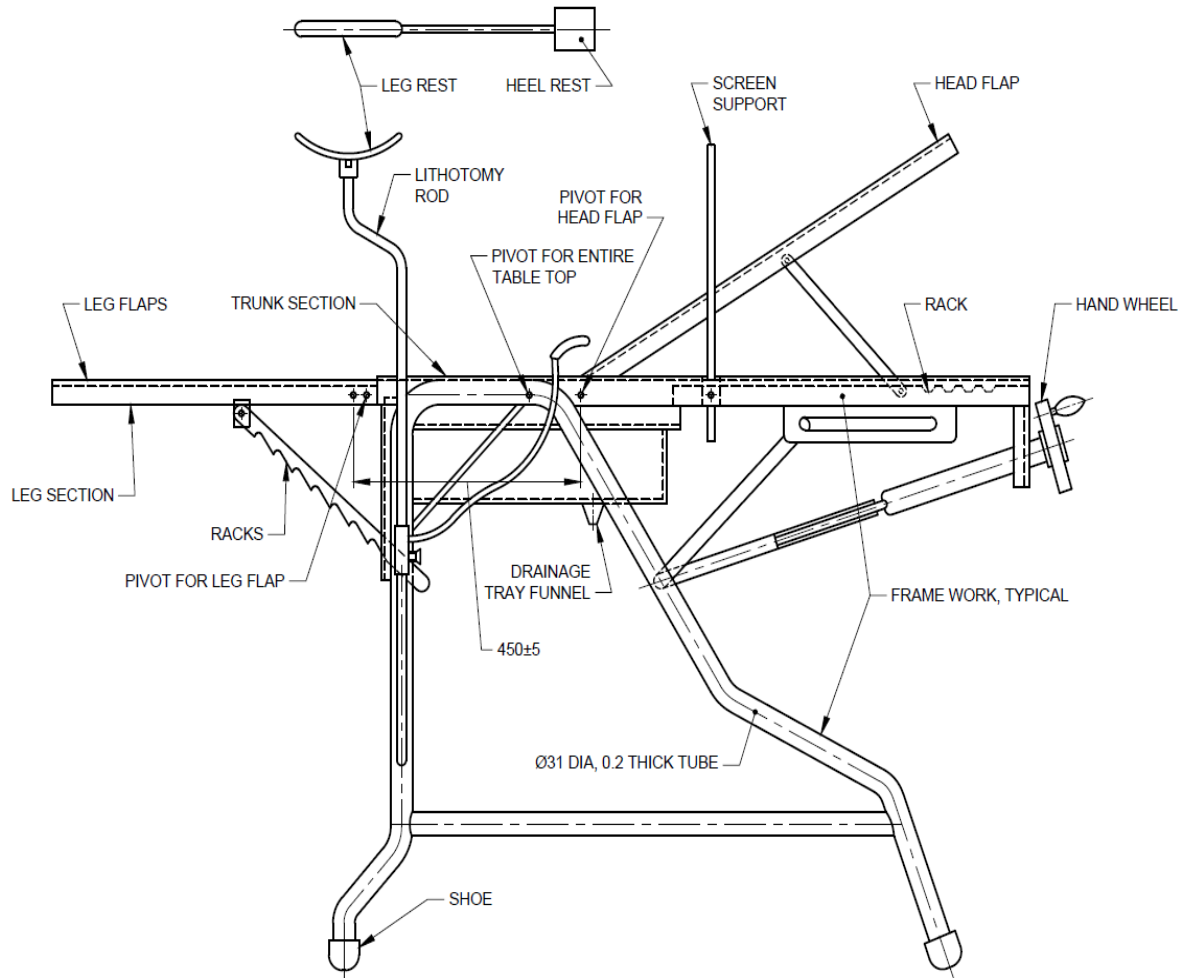

All Dimensions in Millimetres

Fig. 1 GENERAL PURPOSE NON-HYDRAULIC OPERATION TABLE

TABLE 1 DIMENSIONS OF OPERATION TABLE

<i>Part</i>	<i>Dimensions in mm</i>
Length	1800±5
Width	500 to 510
Height	865 to 875
Table top	1.25±0.05 thick

6 CONSTRUCTION REQUIREMENTS

6.1 Framework

The framework of continuous lengths of mild steel tubes (*see* Fig. 1) shall be welded to give the desired shape. The floor ends of the tubular framework shall be fitted with metal shoes with rounded edges.

6.2 Table Top

The table top shall have a minimum of three sections that is head, trunk and leg section. The leg section may have one or two flaps as required by the purchaser and manufacturer. The entire top shall be capable of satisfying the following requirements:

- The entire table top shall be capable of being tilted to 30° Trendelenburg and 20° for reverse Trendelenburg Positions.

- b) The head end shall be capable of being raised by 60° and the leg end to be capable of dropping by 90°.
- c) The table top shall be provided with a perineal cut-out for drainage tray.

6.2.1 Head and Leg Sections

The head section shall be capable of being raised to 60° from the trunk position. The two flaps of the leg section shall be capable of being lowered to at least 90° from the trunk to enable the table top to be used as a chair and also for obtaining other positions. The head and leg sections shall have an operating mechanism situated in such a way that it shall not interfere with the surgical team. The controls for the head and leg ends shall be on the respective ends.

7 ACCESSORIES

7.1 The table shall be provided with two lithotomy rods which are chromium plated conforming to **Service Condition 2** of IS 1068.

7.2 The following accessories shall be optional:

TABLE 2 LIST OF ACCESSORIES

<i>Sr No.</i>	<i>Accessories</i>	<i>Count in Nos.</i>
i)	Leg rests	2
ii)	Screen support	1
iii)	Rubber mattress 25 mm thick, having antistatic properties with resistance between 10 ohms and 10 ⁶ ohms	1
iv)	Heels rests	2

8 PERFORMANCE REQUIREMENTS

8.1 Base

The construction of the table shall ensure stability of the base. The metal framework shall have four metal shoes to provide sufficient rigidity to the table.

8.2 Table Top

The table top shall have requirements as given below:

- a) The extreme edge of the head section shall be applied with a vertical load of 500N, when the load is applied the leg section shall not lift by more than 10 mm.
- b) The load of 250 N is dropped from a height of 150 mm on the extreme end of the 2 leg flaps, when the load is applied the flaps shall not get dislodged.
- c) There shall be no wobble under normal working conditions when the accessories are clamped.

9 TESTING REQUIREMENTS

9.1 Adhesion Test

The adhesion test required for the operation table shall conform to **6.1.1** of IS 4033.

10 WORKMANSHIP AND FINISH

10.1 The operation table components shall provide smooth operation and additional performance requirements as per **8**. The operation table surfaces shall be well finished and free from surface defects, such as pinholes, blisters, blow-holes and similar other defects. The edges shall be rounded off and the three sections comprising the table top in their normal position shall be in one plane when tested with a spirit level. The sweeps of the head and leg sections shall be easy. The welded joints shall have welds fully penetrating and well finished. The minor operation table metal surfaces shall be non-corrosive (aluminium and stainless steel) with matt finish.

10.2 The corrosive surface like steel castings for base, cylinder casings, foot pedals shall be painted to shades such as sea green or low reflective shades agreed to between the manufacturer and the purchaser. Initially the surface which is painted shall be degreased, rust-proofed by phosphating and then suitably protected by an anti-corrosive primer with brushing or spraying and then finished by spraying in stove enamel or air-drying enamel of the specified shade. The procedure on each stage shall be separately stoved or air-dried.

10.3 The resulting finish shall be hard and shall not readily chip or flake. The mild steel and brass parts shall be plated chromium over nickel according to **Service Condition 2** of IS 1068.

11 MARKING

11.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the Identification mark of the manufacturer.

11.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

12 OPERATION MANUAL

12.1 The operation table shall be provided with instruction manual with following information:

- a) Brief instructions for installation and maintenance (including spare parts);
- b) Any other information considered necessary by the manufacturer.

13 PACKAGING

The operation table shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one unit and may be marked with the name of the item, and identification of the source of manufacture and batch number and any other marking if so desired.