

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
मेयो प्रकार का उपकरण रखने के लिए मेज - विशिष्टि
[IS 6905 का पहला पुनरीक्षण]

Draft Indian Standard
Mayo Instrument Table - Specification
[First Revision of IS 6905]

ICS 11.140

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1973. The first revision of this standard has been brought out to align it with recent developments in the material requirements and to bring the standard in line with the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 'Rules for rounding off numerical values (*second revision*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies the dimensional and other requirements for Mayo instrument table used in hospitals and other similar institutions.

2 REFERENCES

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
MHD 12 (33411) WC (Under Development)	Hospital Furniture - General Requirements (<i>first revision</i>)
IS 1068: 2025 ISO 1456: 2009	Metallic and other inorganic coatings - Electrodeposited coatings of nickel, nickel plus chromium, copper plus nickel and of copper plus nickel plus chromium (<i>fourth revision</i>)
IS 1868:1996	Anodic coatings on aluminium and its alloys - Specification (<i>third revision</i>)
IS 17523: 2021	Castors and Wheels - Requirements for Castors for Furniture

3 TERMINOLOGY

3.1 Mayo Instrument Table - The small, mobile, and height-adjustable table stand which is designed to hold frequently used sterile instruments and supplies within direct and immediate reach of the surgeon during a procedure.

4 MATERIAL REQUIREMENTS

4.1 Framework

The material used for the framework shall be as per **3.1** of IS 4033.

4.2 Rod

The rod used for instrument table top shall be made from mild steel or aluminium alloy of suitable composition.

4.3 Top


The top of the instruments table shall be in accordance with **3.2(a)**, **3.2(b)** and **3.2(c)** of IS 4033.

4.4 Castors

The castor which is used for the instrument table shall conform to the requirements as per IS 17523.

5 SHAPE AND DIMENSIONS

5.1 The shape and dimensions of the instrument table shall be as given in Fig. 1.

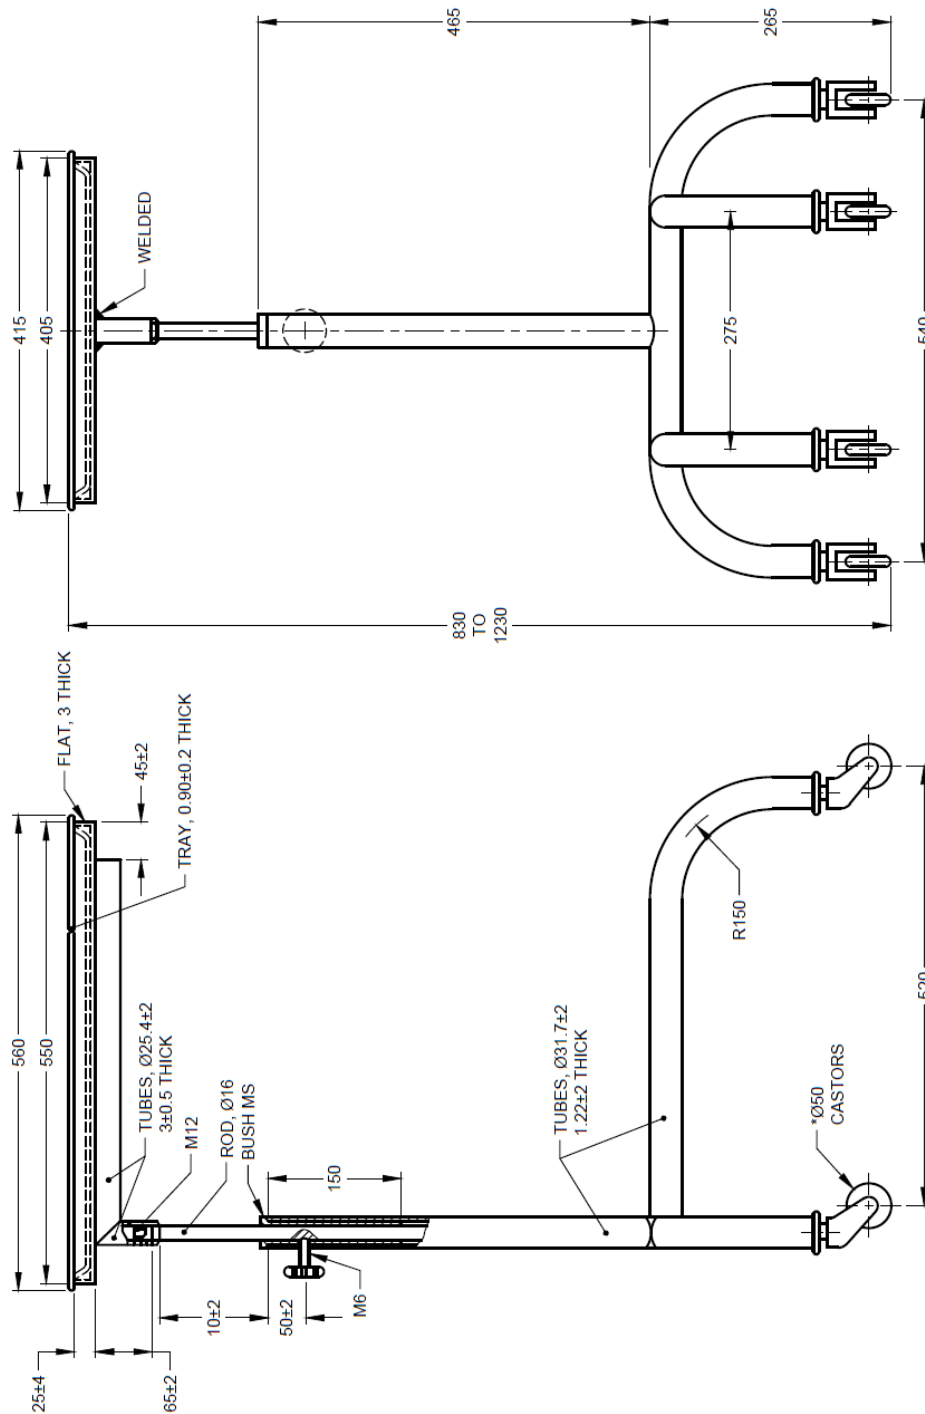

Tolerance on all dimensions ± 5 mm except where specified

All dimensions in millimetres.

Fig. 1 MAYO INSTRUMENT TABLE

6 CONSTRUCTION REQUIREMENTS

6.1 Framework

The table shall have a framework of tubes as per Fig. 1. The framework shall have four castors for the smooth movement of the table.

6.2 The stem of the table shall have a movable arrangement for raising and lowering the table top. The stem shall have a locking arrangement by providing holes for heights between 830 to 1230 mm.

6.3 The sheet metal top of the table shall be welded to the stem tube at right angles to each other. The additional arrangement for fixing the top shall be as agreed to between the purchaser and the manufacturer.

6.4 The removable type of tray shall have handles on both sides and it is placed on the metal top as per Fig. 1.

6.5 The additional details for the instrument table shall be according to **5.1** of IS 4033.

6.6 Castors

The instrument table provided with castors shall be made from antistatic rubber tread conform to IS 17523. The castors shall have locking arrangements to protect the movement of table. The additional requirements shall be as per **5.2** of IS 4033.

7 TESTING REQUIREMENTS

7.1 Adhesion Test

The adhesion test required for the instrument table shall conform to **6.1.1** of IS 4033.

7.2 Performance Test

The performance test for the instrument table shall be as per **6.1.2** of IS 4033 which is tested by putting additional load.

8 WORKMANSHIP AND FINISH

8.1 The rod of the movable arrangement on which the table top is mounted shall be made from mild steel which is plated with chromium over nickel in accordance with **Service Condition 2** of IS 1068 or made of aluminium alloy which shall be anodized in accordance with IS 1868 or made of stainless steel which shall be passivated.

8.2 The components of the instrument table shall be painted in accordance with **7.1** of IS 4033.

8.3 The inside bore of the stem and locking lug shall be free from burrs and sharp edges to allow the rod to operate smoothly.

9 MARKING

9.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the Identification mark of the manufacturer.

9.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

10 PACKAGING

The instrument table shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one unit and may be marked with the name of the item, and identification of the source of manufacture and batch number and any other marking if so desired.