

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
दवाइया रखने के लिए पहियेदार मेज - विशिष्टि
[IS 7083 का पहला पुनरीक्षण]

Draft Indian Standard
Medicine Trolley - Specification
[First Revision of IS 7083]

ICS 11.140

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1973. The first revision of this standard has been brought out to align it with recent developments in the material requirements, addition of workmanship and finish and to bring the standard in line with the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 'Rules for rounding off numerical values (*second revision*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies the dimensional and other requirements for medicine trolley used in hospitals and other similar institutions.

2 REFERENCES

The standards listed in **Annex A** contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

3 MATERIAL REQUIREMENTS

3.1 Framework

The material used for the framework shall be as per **3.1** of IS 4033.

3.2 Shelves

The shelves used in the medicine trolley shall be made from materials specified in **3.2 (a) to 3.2 (c)** of IS 4033.

3.3 Railings

The railings used in the medicine trolley shall be made from mild steel strips in accordance with IS 513 (Part 2) or IS 1029 or mild steel tube of 15 mm diameter as per IS 1239 (Part 1).

3.4 Domed Caps


The domed caps used for closing the framework tubing which shall be made up of mild steel or aluminium or PVC.

3.5 Bowls

The bowls used in medicine trolleys shall be made from stainless steel conforming to designation X07Cr18Ni9 of IS 6911.

4 SHAPE AND DIMENSIONS

The shape and dimensions of the medicine trolley shall be as given in Fig. 1.

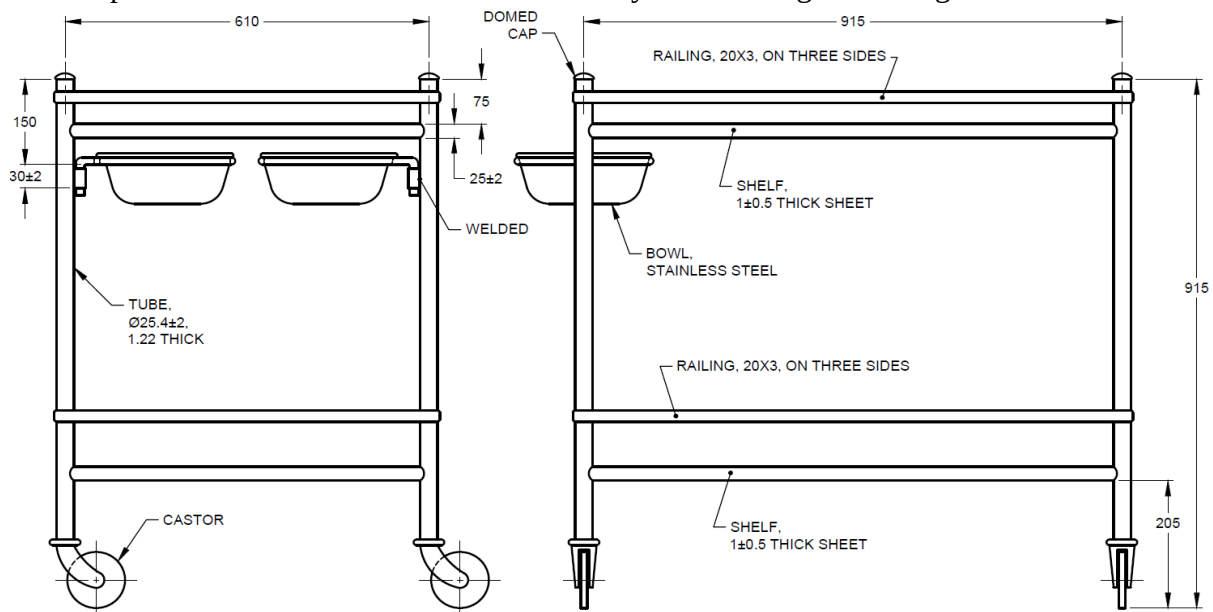

Tolerance on all dimensions ±5 mm

All dimensions in millimetres

Fig. 1 MEDICINE TROLLEY

5 CONSTRUCTION REQUIREMENTS

5.1 The medicine trolley shall have a welded framework of continuous lengths of mild steel tube as shown in Fig. 1.

5.2 The shelves and the railings used in the medicine trolley shall be welded to the upright members.

5.3 The upper ends of the upright members shall be fitted with domed caps.

5.4 The medicine trolley shall be fitted with castors conforming to IS 17523.

5.4.1 The wheels of the castors shall have antistatic rubber tread or alternatively the construction of the medicine trolley shall be such as to ensure transmission of static charge to the earth.

5.5 The medicine trolley shall be provided with two stainless steel bowls which shall rest on rings hinged to the upright members as per Fig. 1.

6 TESTING REQUIREMENTS

6.1 Adhesion Test

The adhesion test required for the medicine trolley shall conform to **6.1.1** of IS 4033.

6.2 Performance Test

The performance test for the medicine trolley shall be as per **6.1.2** of IS 4033 which is tested by putting additional load.

6.2.1 The performance test shall be carried out and it is noted that the shelves shall not get displaced or make rattling noise.

7 WORKMANSHIP AND FINISH

7.1 The medicine trolley shall be free from cracks, sharp edges and burrs.

7.2 The finish for the medicine trolley shall be in accordance with **7** of IS 4033. The enamels for the undercoating and finishing coat shall conform to IS 2932.

8 MARKING

8.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the Identification mark of the manufacturer.

8.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

9 PACKAGING

The medicine trolley shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one unit and may be marked with the name of the item, and identification of the source of manufacture and batch number and any other marking if so desired.

ANNEX A

(Clause 2)

LIST OF REFERRED INDIAN STANDARDS

<i>IS No.</i>	<i>Title</i>
MHD 12 (33411) WC (Under Development)	Hospital Furniture - General Requirements (<i>first revision</i>)
IS 513 (Part 2): 2016	Cold reduced carbon steel sheet and strip: Part 2 high tensile and multi - Phase steel (<i>sixth revision</i>)
IS 1029:1970	Specification for hot-rolled steel strip (Baling) (<i>first revision</i>)
IS 1239 (Part 1):2004	Steel tubes, tubulars and other wrought steel fittings - Specification: Part 1 steel tubes (<i>sixth revision</i>)
IS 6911:2017	Stainless steel plate, sheet and strip - Specification (<i>second revision</i>)
IS 2932 (Part 1):2013	Enamel, synthetic, exterior: (a) Undercoating (b) Finishing - Specification : Part 1 For domestic and decorative applications (<i>fourth revision</i>)
IS 17523: 2021	Castors and Wheels - Requirements for Castors for Furniture