

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
चिकित्सा सामग्री का डिब्बा रखने के लिए पहियेदार मेज - विशिष्टि
[IS 7099 का पहला पुनरीक्षण]

Draft Indian Standard
Dressing Drum Trolley - Specification
[First Revision of IS 7099]

ICS 11.140

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1973. The first revision of this standard has been brought out to align it with recent developments in the material requirements, addition of tolerance and to bring the standard in line with the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 'Rules for rounding off numerical values (*second revision*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies the dimensional and other requirements for the dressing drum trolley used in hospitals and other similar institutions.

2 REFERENCES

The standards listed in **Annex A** contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

3 MATERIAL REQUIREMENTS

3.1 Framework

The framework shall be electric-resistance fusion-welded steel tube conforming to IS 2039 (Part 2).

3.2 Rings


The rings used in the trolley shall be made from mild steel wire as per IS 280.

3.3 Pedals, Foot Operated Lever Mechanism and Drum Support

The steel parts used for pedals, foot lever and drum support shall conform to IS 513 (Part 2) and IS 1029.

4 SHAPE AND DIMENSIONS

The shape and dimensions of the dressing drum trolley shall be as given in Fig. 1.

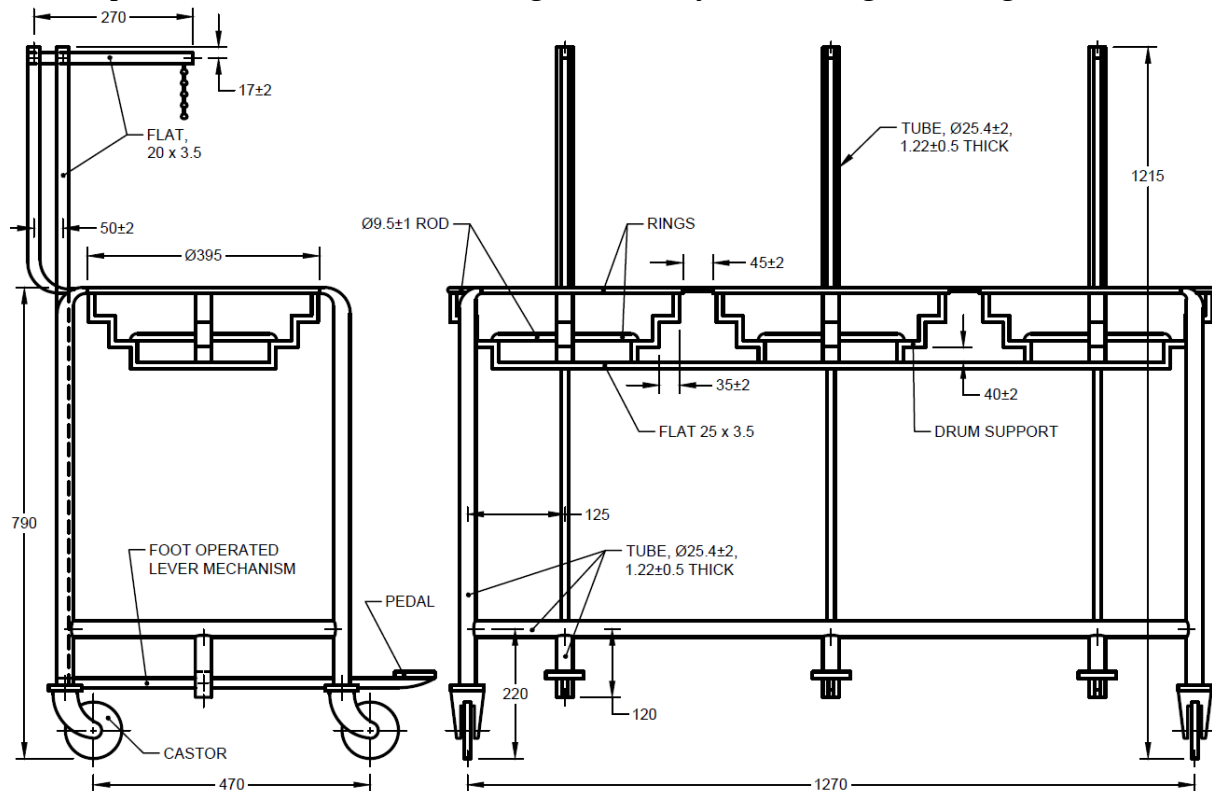

Tolerance on all dimensions ±5 mm except where specified

All dimensions in millimetres.

Fig. 1 DRESSING DRUM TROLLEY

5 CONSTRUCTION REQUIREMENTS

5.1 The dressing drum trolley shall have a welded framework of continuous lengths of mild steel tube as per IS 819 and IS 1323.

5.2 The parts that are assembled by welding shall be fully penetrated.

5.3 The trolley shall be capable of occupying three sizes of dressing drums.

5.4 The trolley shall be equipped with foot-operated lever mechanism which is capable of opening and closing the lids of the dressing drum, the lever mechanism shall be separate for each dressing drum arrangement.

5.5 The foot lever shall be operated by pedals which are provided with caps made of plastics, rubber or other resilient material.

5.6 The dressing drum trolley shall be fitted with castors conforming to IS 17523.

6 TESTING REQUIREMENTS

6.1 Adhesion Test

The adhesion test required for the dressing drum trolley shall conform to **6.1.1** of IS 4033.

6.2 Performance Test

The performance test for the dressing drum trolley shall be as per **6.1.2** of IS 4033 which is tested by putting additional load.

7 WORKMANSHIP AND FINISH

7.1 The welding places shall be well finished and there shall not be exposed sharp edges or unsealed formations.

7.2 The dressing drum trolley shall be free from dents, burrs and sharp edges.

7.3 The trolley shall be painted in accordance with **7.1** of IS 4033. The enamels for the undercoat and finishing coat shall be as per IS 2932.

8 MARKING

8.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the Identification mark of the manufacturer.

8.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

9 PACKAGING

The dressing drum trolley shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one unit and may be marked with the name of the item, and identification of the source of manufacture and batch number and any other marking if so desired.

ANNEX A

(Clause 2)

LIST OF REFERENCED INDIAN STANDARDS

<i>IS No.</i>	<i>Title</i>
IS 2039 (Part 2): 1991	Steel tubes for bicycle and cycle rickshaws - Specification (<i>second revision</i>)
IS 513 (Part 2): 2016	Cold reduced carbon steel sheet and strip: Part 2 high tensile and multi - Phase steel (<i>sixth revision</i>)
IS 1029:1970	Specification for hot-rolled steel strip (Baling) (<i>first revision</i>)
MHD 12 (33411) WC (Under Development)	Hospital Furniture - General Requirements (<i>first revision</i>)
IS 280: 2006	Mild steel wire for general engineering purposes (<i>fourth revision</i>)
IS 819: 1957	Code of practice for resistance spot welding for light assemblies in mild steel
IS 1323:1982	Code of practice for Oxy - Acetylene welding for structural work in mild (<i>second revision</i>)
IS 2932 (Part 1):2013	Enamel, synthetic, exterior: (a) Undercoating (b) Finishing - Specification : Part 1 For domestic and decorative applications (<i>fourth revision</i>)
IS 17523: 2021	Castors and Wheels - Requirements for Castors for Furniture