

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
प्रसूति प्रसव के लिए मेज - विशिष्टि
[IS 6083 का पहला पुनरीक्षण]

Draft Indian Standard
Obstetric Labour Table - Specification
[First Revision of IS 6083]

ICS 11.140

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1971. The first revision of this standard has been brought out to align it with recent developments in the material requirements and to bring the standard in line with the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 'Rules for rounding off numerical values (*second revision*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies the dimensional and construction requirements for an obstetric labour table used in hospitals and other similar institutions.

2 REFERENCES

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
MHD 12 (33411) WC (Under Development)	Hospital Furniture - General Requirements (<i>first revision</i>)
IS 6911: 2026	Stainless Steel Plate, Sheet and Strip - Specification (<i>third revision</i>)
IS 17523: 2021	Castors and Wheels - Requirements for Castors for Furniture

3 TERMINOLOGY

3.1 Obstetric Labour Table - The specialized medical bed designed to provide support and adjustability for a patient during childbirth.

4 MATERIAL REQUIREMENTS

4.1 Framework

The material used for the framework shall be as per **3.1** of IS 4033.

4.2 Top

The top used for the table shall be as per **3.2 (a)** of IS 4033.

4.3 Channel Support


The channel support shall be made up of mild steel which is either cold rolled or hot rolled quality.

4.4 Lithotomy Rods

The lithotomy rods which are used for the table shall be made up of stainless-steel designation X07Cr17Ni12Mo2 in accordance with IS 6911.

5 SHAPE AND DIMENSIONS

The shape and dimensions of the table shall be as per Fig. 1.

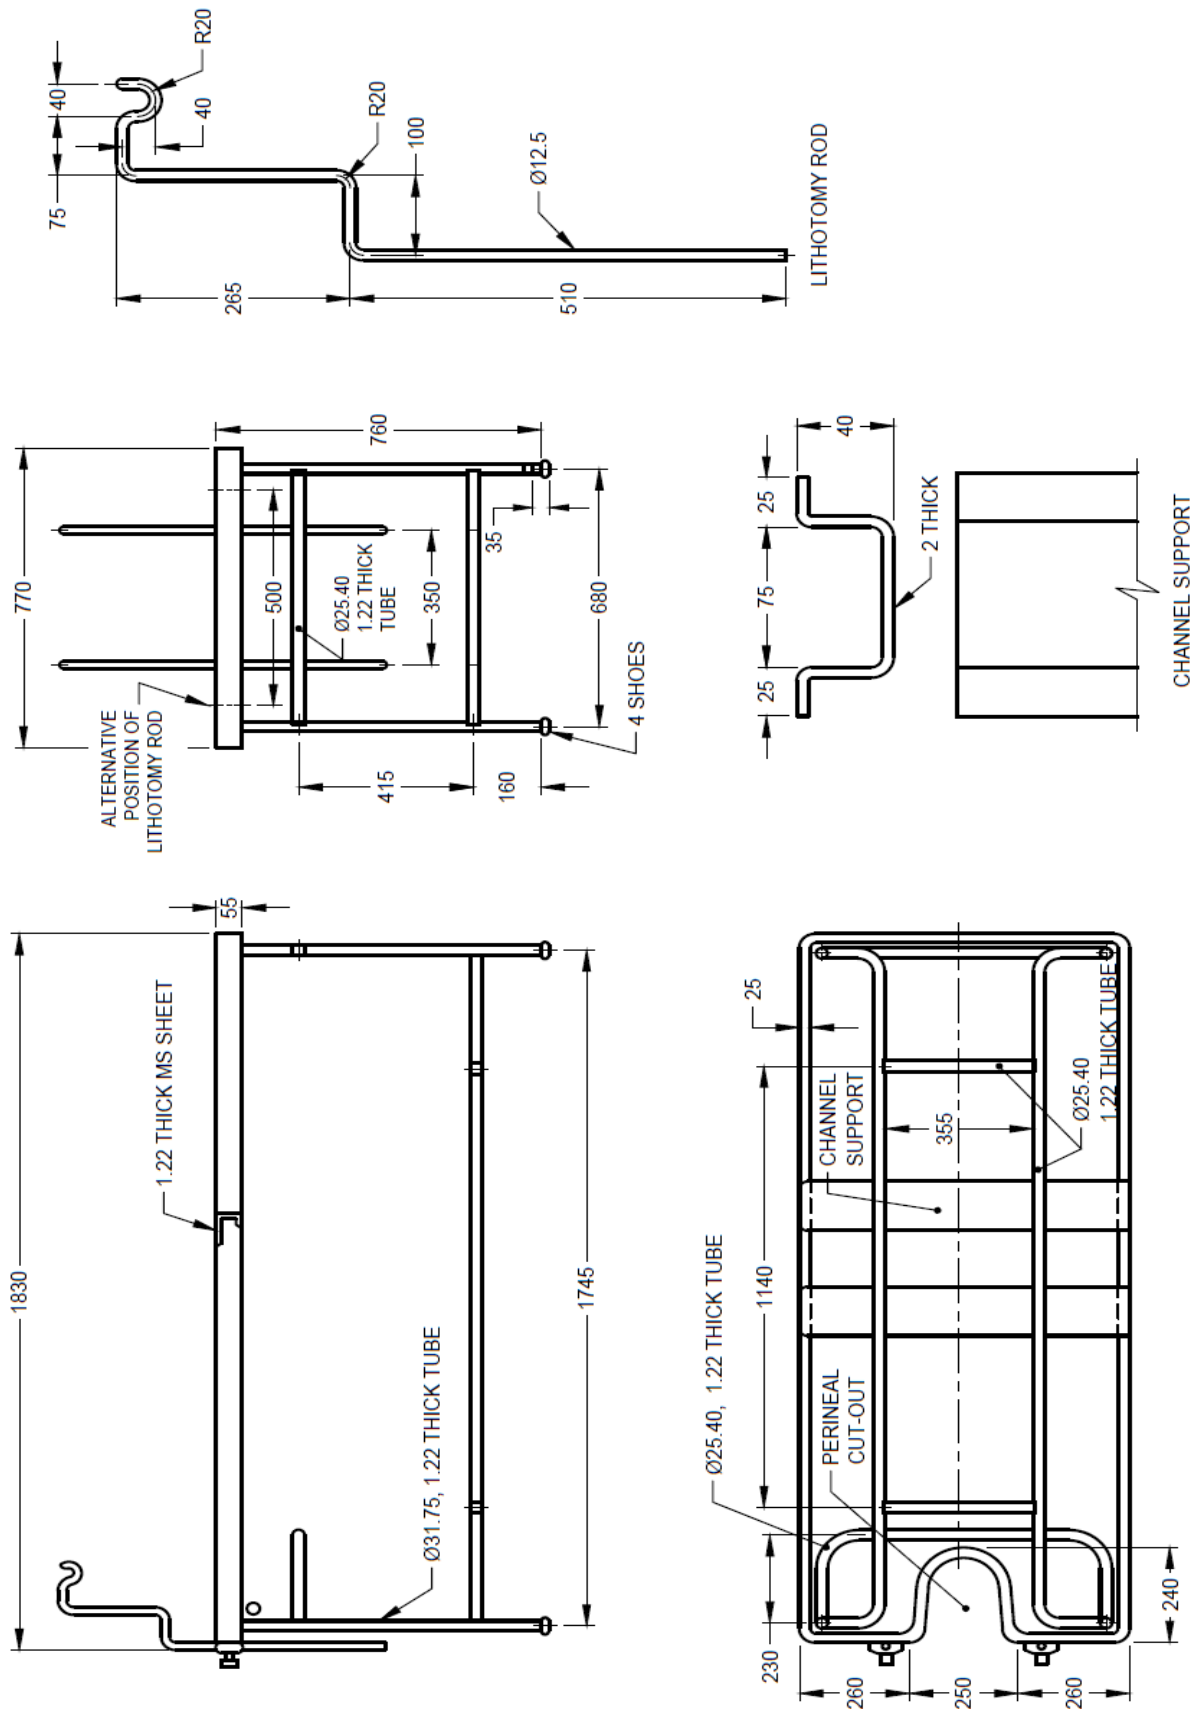

Tolerance on all dimensions ± 5 mm

All dimensions in millimetres

Fig. 1 OBSTETRIC LABOUR TABLE

6 CONSTRUCTION REQUIREMENTS

6.1 Framework

The obstetric labour table shall have a welded framework of continuous lengths of angle iron of size 40 mm × 40 mm × 3 mm. The four upright members shall be connected at the floor end by a pair of longitudinal and a pair of transverse angles. The upright members shall support a formed metal top with a perineal cut-out. The arrangement for welding the sheet metal tops and the upright member shall be sturdy and sound. The perineal cut-out side of the table shall have arrangement for receiving two lithotomy rods which shall be designed to provide rigid support. The table shall be free from burrs and sharp edges. The floor ends of the uprights shall be fitted with aluminium shoes. Additionally, a drainage pipe shall be provided. The top of the table shall have a slope to facilitate drainage into the drain hole.

7 TESTING REQUIREMENTS

7.1 Adhesion Test

The adhesion test required for the table shall conform to **6.1.1** of IS 4033.

8 WORKMANSHIP AND FINISH

The finish for the table shall be in accordance with **7** of IS 4033.

9 MARKING

9.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the Identification mark of the manufacturer.

9.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act*, 2016 and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

10 PACKAGING

The table shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one unit and may be marked with the name of the item, and identification of the source of manufacture and batch number and any other marking if so desired.