

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
सामान्य औषध भंडार के लिए पहियेदार मेज - विशिष्टि
[IS 9133 का पहला पुनरीक्षण]

Draft Indian Standard
General Medical Store Trolley - Specification
[First Revision of IS 9133]

ICS 11.140

Hospital Equipment and Surgical Disposable
Products Sectional Committee, MHD 12

Last date for comments:
12 September 2026

FOREWORD

(Formal clause will be added later)

This standard was originally published in 1979. The first revision of this standard has been brought out to align it with recent developments in the material requirements and to bring the standard in line with the latest style and format of referred standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2: 2022 'Rules for rounding off numerical values (*second revision*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This standard specifies the dimensional and other requirements for the general medical store trolley.

2 REFERENCES

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

<i>IS No.</i>	<i>Title</i>
MHD 12 (33411) WC (Under Development)	General requirements for hospital furniture (<i>first revision</i>)
IS 17523: 2021	Castors and Wheels- Requirements for Castors for Furniture

3 MATERIAL REQUIREMENTS

3.1 Framework

The framework shall be as per 3.1 of IS 4033.

3.2 Angles

The angles used in the trolley shall be made from mild steel.

3.3 Castors

The castors used for trolley shall be in accordance with IS 17523.


4 SHAPE AND DIMENSIONS

4.1 The shape and dimensions of the medical store trolley shall be as given in Table 1 and Fig. 1.

4.2 The medical store trolley shall be provided with dimensions for large and small size.

Table 1 DIMENSIONS OF LARGE AND SMALL TYPE MEDICAL STORE TROLLEY

<i>Type</i>	<i>A</i>	<i>B</i>	<i>C</i>
Large	1215	650	155
Small	900	600	450

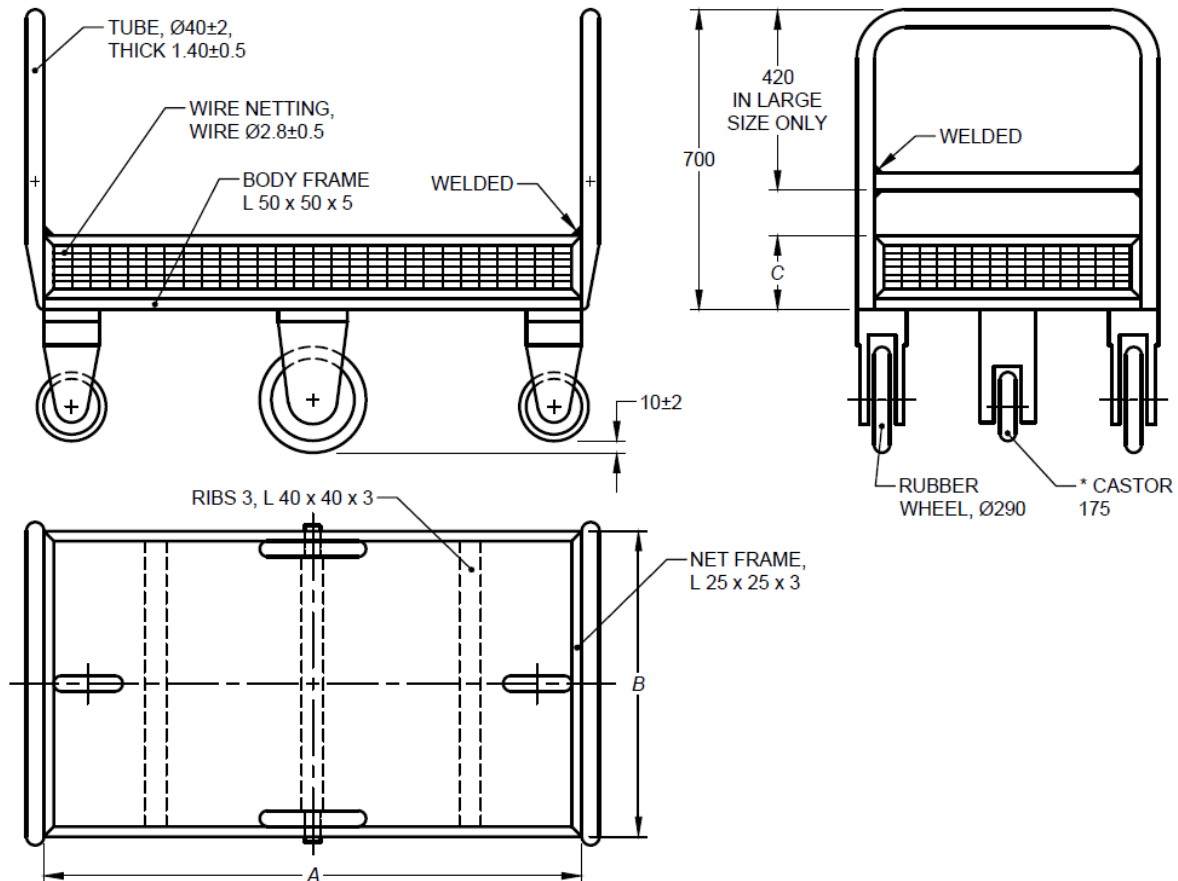

*Tolerance on all dimensions ±10 mm
All dimensions in millimetres*

Fig. 1 MEDICAL STORE TROLLEY

5 CONSTRUCTION REQUIREMENTS

5.1 Handle

The handle used for the trolley shall be manufactured from a stainless-steel tube bent and welded as per Fig. 1.

5.2 Frame

The frame shall be made from mild steel angles. The mild steel sheet shall be of 1.25 mm thickness which is fixed at the bottom of the trolley. The sides of trolley shall be provided with brackets for wire mesh or panel installation as agreed between manufacturer and purchaser to provide protective height for trolley. The trolley castor shall be tack welded to the trolley.

6 TESTING REQUIREMENTS

6.1 Adhesion Test

The adhesion test required for the medical store trolley shall conform to **6.1.1** of IS 4033.

6.2 Performance Test

The performance test for the medical store trolley shall be as per **6.1.2** of IS 4033. The trolley is tested by putting an additional load of 150 Kg for larger-sized trolley and 100 Kg for the smaller-sized trolley.

7 WORKMANSHIP AND FINISH

7.1 The welds at the welding places shall be fully penetrating. The welding places shall not have exposed sharp edges or unsealed formations.

7.2 The medical store trolley shall be smooth and well finished as per **7** of IS 4033.

7.3 The trolley shall be painted in accordance with **7.1** of IS 4033.

8 MARKING

8.1 The marking which is used by the manufacturer shall be legibly and indelibly marked with the Identification mark of the manufacturer.

8.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act*, 2016 and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

9 PACKAGING

The medical store trolley shall be packed as agreed to between the purchaser and the manufacturer. Each individual package shall contain only one unit and may be marked with the name of the item, and identification of the source of manufacture and batch number and any other marking if so desired.