

BUREAU OF INDIAN STANDARDS

DRAFT FOR COMMENTS ONLY

(Not to be reproduced without permission of BIS or used as an Indian Standard)

भारतीय मानक मसौदा
पशु चिकित्सा सर्जिकल उपकरण — टूथ रैस्प प्रतिवर्ती
— विशिष्टि

(IS 12243 का पहला पुनरीक्षण)

Draft Indian Standard

**Veterinary Surgical Instruments — Tooth Rasp
Reversible— Specification**

(First Revision of IS 12243)

ICS 11.220

Veterinary Hospital Planning and Surgical
Instruments Sectional Committee, MHD 13

Last date for comments: **14 September 2026**

FOREWORD

(Formal clauses will be added later)

This Indian Standard was first published in 1988 as ‘Specification for rasp, tooth, reversible’. The first revision of this standard has been brought out to align the cross references to the latest standards.

For the purpose of deciding whether a particular requirement of this standard is complied with the final value, observed or calculated, expressing the result of a test or analysis shall be rounded off in accordance with IS 2 : 2022 ‘Rules for rounding off numerical values (second revision)’. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

1 SCOPE

This Indian Standard covers the requirements for set of three pieces of tooth rasp, reversible, for veterinary use.

2 REFERENCES

The standards given below contain provisions which, through reference in this text, constitute provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of these standards.

IS No.	Title
IS 2102 (Part 1) : 1993	General Tolerances Part 1 Tolerances for Linear and Angular Dimensions Without Individual Tolerance Indications (<i>third revision</i>)
IS 2500 (Part 1) : 2000	Sampling procedures for inspection by attributes: Part 1 sampling schemes indexed by acceptance quality limit (AQL) for lot - By - Lot inspection (<i>third revision</i>)
IS 3748 : 2022	Tool Steels – Specification (<i>Third Revision</i>)

3 MATERIAL

Shall conform to designation C120U of IS 3748.

4 SHAPE AND DIMENSIONS

4.1 Shall Conform to Fig. 1.

4.2 The tolerance on dimensions of working ends shall conform to ‘fine’ class of deviation and the tolerance for remaining dimensions shall conform to ‘medium’ class of deviation of IS 2102 (Part 1).

5 MANUFACTURE WORKMANSHIP AND FINISH

5.1 The surfaces of the rasps except for the tines and threads shall be smooth and free from pitting. The edges shall be even and rounded. The tines shall be well formed. The form and pitch of the threads shall be correct. The male part of rasp shall screw accurately into the female parts of rasp. The male rasp of one set shall fit accurately into the female rasps of any other set in the same supply and *vice versa*.

5.2 The surface of the working ends shall be free from all defects like burrs, pits, cracks, nicks and waviness when examined under x 10 magnification. All surfaces shall be free from pores, crevices and grinding marks.

5.3 The rasps shall be supplied free from residual scales, acid, grease and grinding and polishing materials. Compliance with these requirements shall be checked under x 2 magnification.

6 HARDNESS

Rasp shall be accurately and evenly hardened and tempered to give a hardness of 650 to 750 HV.

7 TESTS

Each rasp piece shall be used for filing the teeth on a horse jaw bone continuously for two minutes. The rasp shall be able to do it easily. On completion of the test, the tines on the rasp shall not show any sign of wear.

8 SURFACE FINISH

The surface finish shall be mirror finish. The instrument should be adequately ground to remove all surface imperfections and polished to remove grinding marks, resulting in a mirror finish. The mirror finish should be effected by an appropriate procedure, such as polishing, brushing, electropolishing and mirror buffing.

9 SAMPLING

9.1 Unless otherwise agreed to between the purchaser and the supplier, the sampling procedure given in IS 2500 (Part 1) shall be followed.

9.2 Lot

All tooth rasps of the same size, shape and belonging to the same batch of manufacture shall be grouped together to constitute a lot.

9.3 For dimensions and requirements given in 4, 5 and 8, a single sampling plan with general inspection level II and AQL 4 percent given in Tables 1 and 2-A of IS 2500 (Part 1) shall be followed.

9.4 For the requirement given in 6, a single sampling plan with special inspection level S-3 and AQL 1 percent given in Tables 1 and 2-A of IS 2500 (Part 1) shall be followed.

10 MARKING


10.1 Each rasp shall be legibly and indelibly marked with the manufacturer's name, initials or recognized trademarks.

10.2 BIS Certification Marking

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the product(s) may be marked with the Standard Mark.

11 PACKING

The set of rasps shall be delivered in a new and clean condition free from all traces of rust. Each rasp shall be coated with a thin film of rust preventing solution and wrapped in normal waxed grade kraft paper. The rasp shall be packed in a set in leather case and tied with a strap. The empty space, if any, shall be filled with suitable cushioning material to prevent movement.

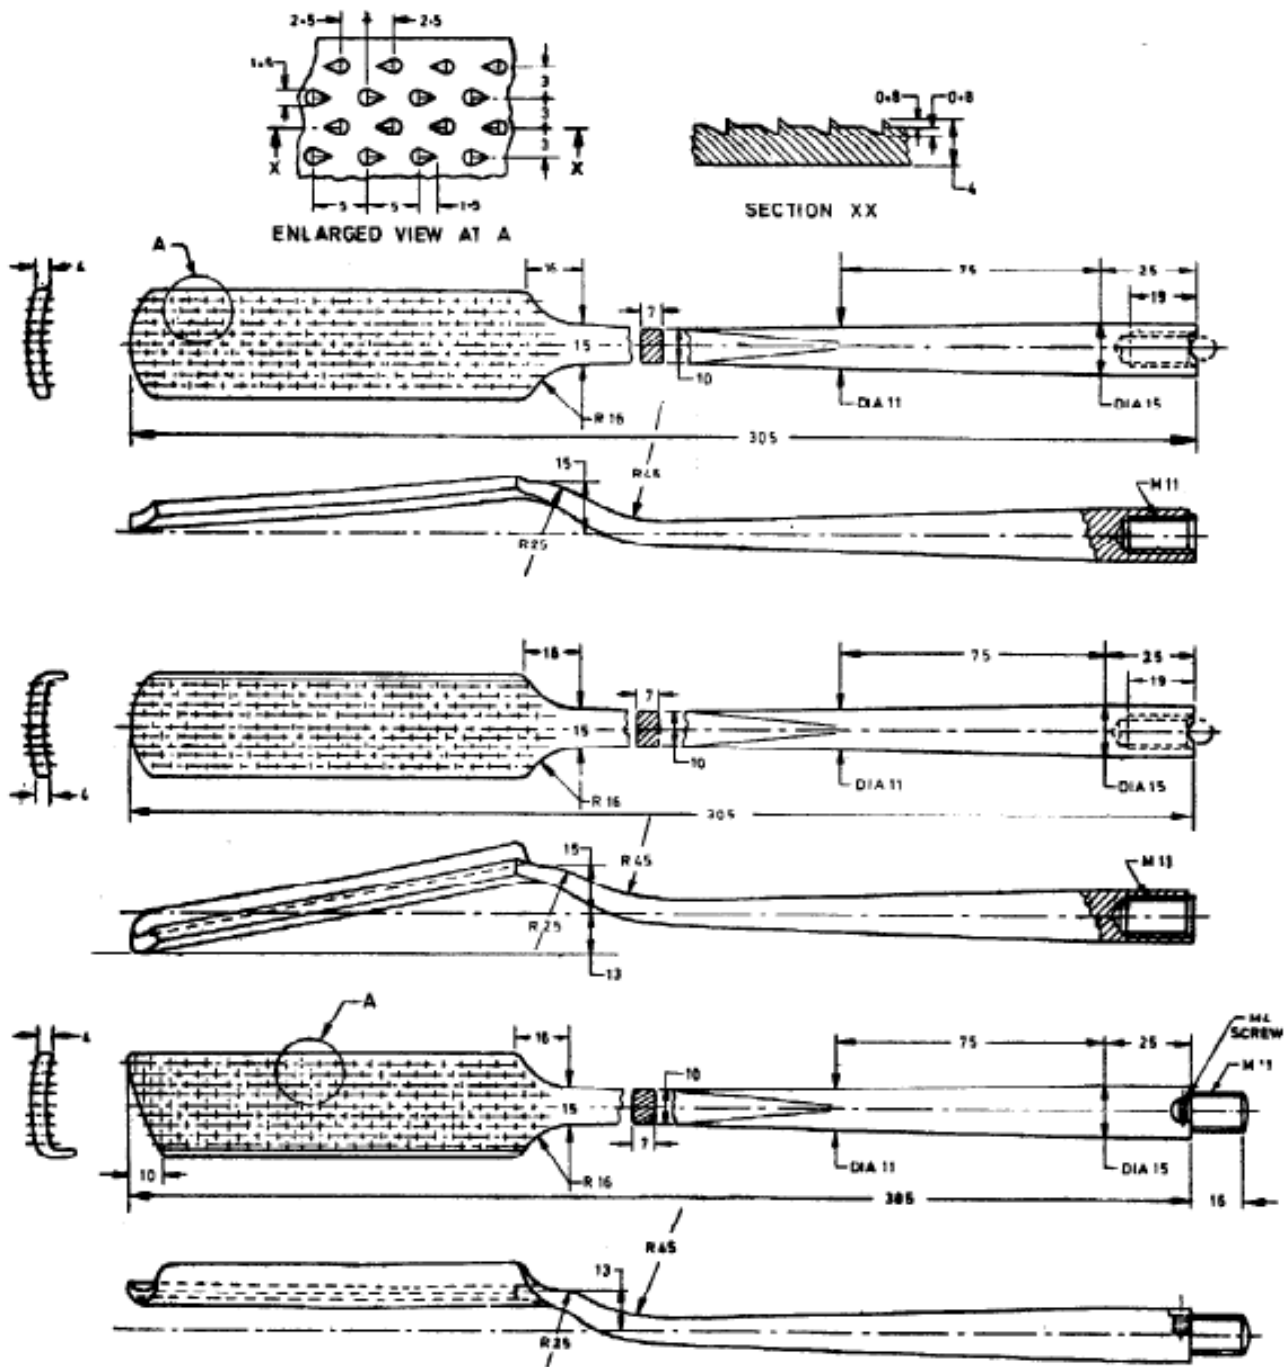

All dimensions in millimetres.

FIG. 1 TOOTH RASP REVERSIBLE