

u^b

b

**UNIVERSITY
OF BERN**

u^b X-ray microtomography

485018-HS2024-0: Advanced Course II
Ultraprecision Engineering

David Haberthür

Institute of Anatomy, September 25, 2024

u^b Grüessech mitenang!

- David Haberthür
 - Physicist by trade
 - PhD in high resolution imaging of the lung, Institute of Anatomy, University of Bern, Switzerland
 - Post-Doc I: TOMCAT, Swiss Light Source, Paul Scherrer Institute, Switzerland
 - Post-Doc II: µCT group, Institute of Anatomy, University of Bern, Switzerland.

u^b

Grüessech from the μ CT-group




David.Haberthuer@unibe.ch

Ruslan.Hlushchuk@unibe.ch

Oleksiy.Khoma@unibe.ch

- microangioCT [1]
 - Angiogenesis: heart, musculature [2] and bones
 - Vasculature: (mouse) brain [3], (human) nerve scaffolds [4], (human) skin flaps [5] and tumors
- Zebrafish musculature and gills [6]
- (Lung) tumor detection and metastasis classification [7]
- Collaborations with museums [8] and scientist at UniBe [9] to scan a wide range of specimens
- Automate *all* the things! [10], [11]

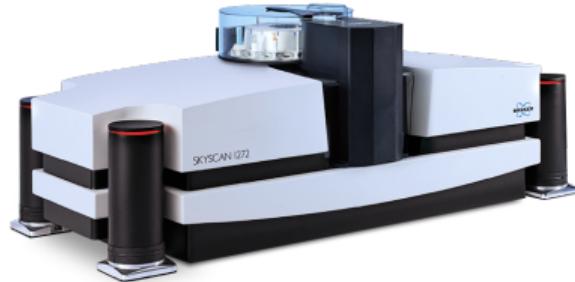

bruker.com/skyscan1272

u^b

Contents

Overview

Imaging

Tomography

Interaction of x-rays with matter

Tomography today

A scan, from *getting started* to *nice image*

Examples

A study about teeth

Overview

Materials & Methods

Results

Metal foam analysis

A study on fish

- Dense and/or non-transparent samples
- Calibrated & isotropic 3D images at micron resolutions
- Covers a very large range of sample sizes
- Gives information at different length scales
- Nondestructive imaging, thus compatible with routine sample preparation.
Enables correlative imaging pipelines, scanning of museum & collection material

u^b

Biomedical imaging


- Medical research
- Non-destructive insights into the samples
- (Small) Biological samples



w.wiki/7g4 CC BY-NC-SA


Biomedical imaging

- Medical research
- Non-destructive in samples
- (Small) Biological

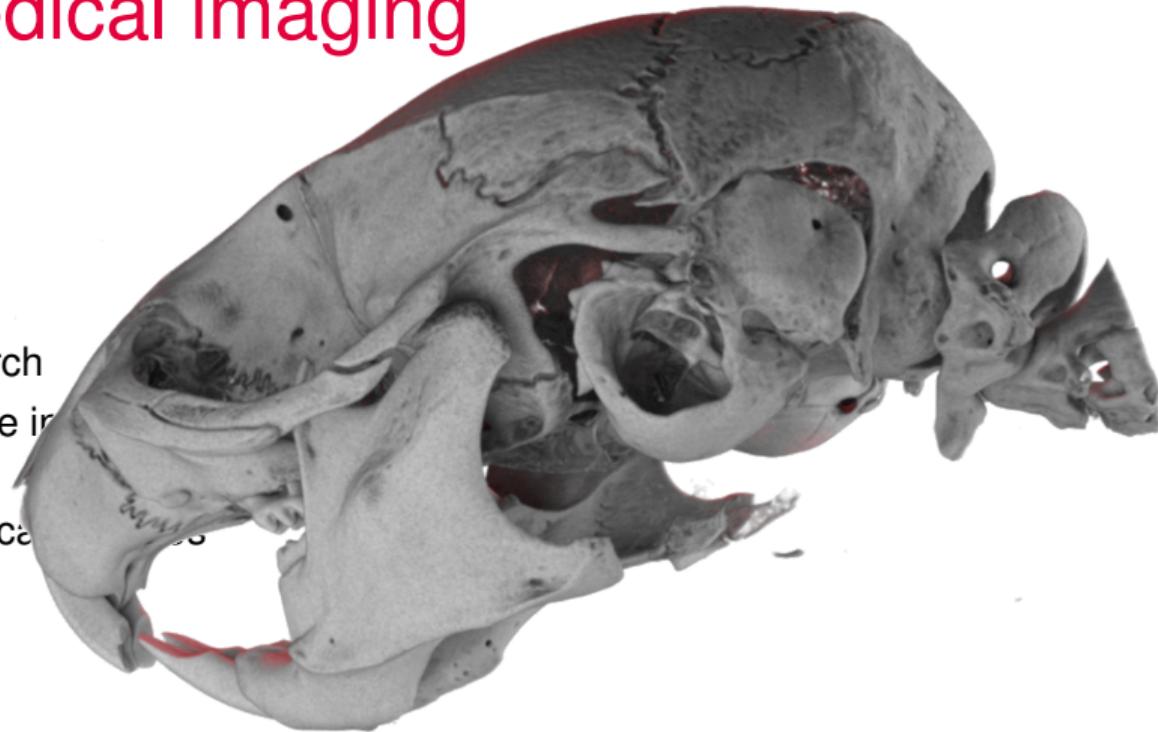


u^b

Wavelength & Scale

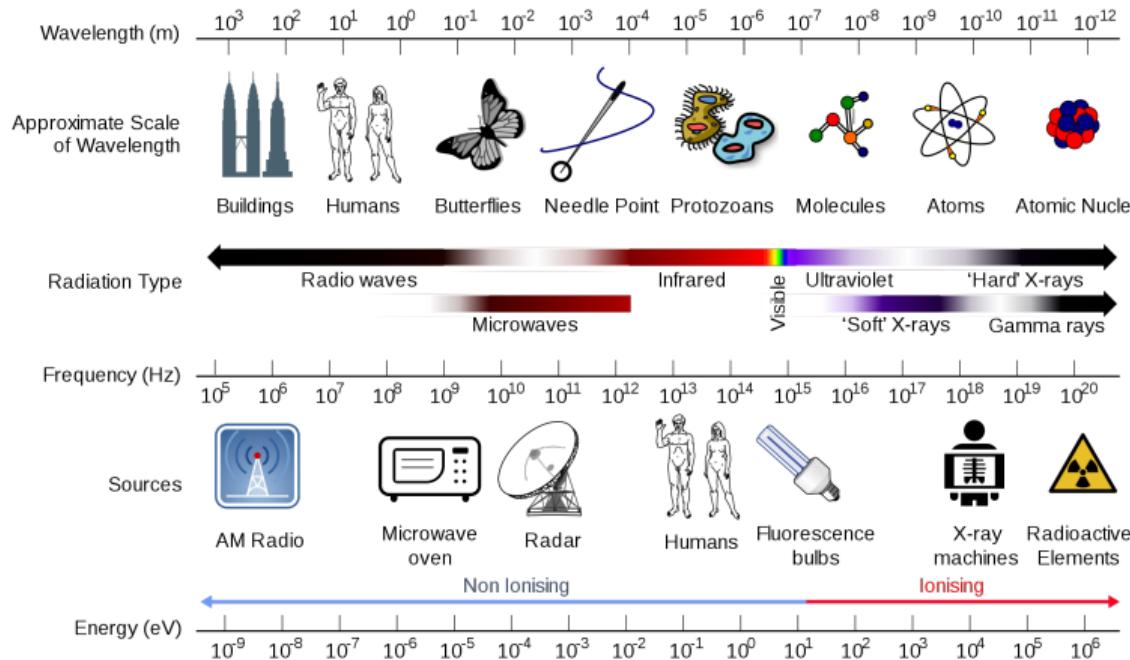

u^b

Wavelength & Scale

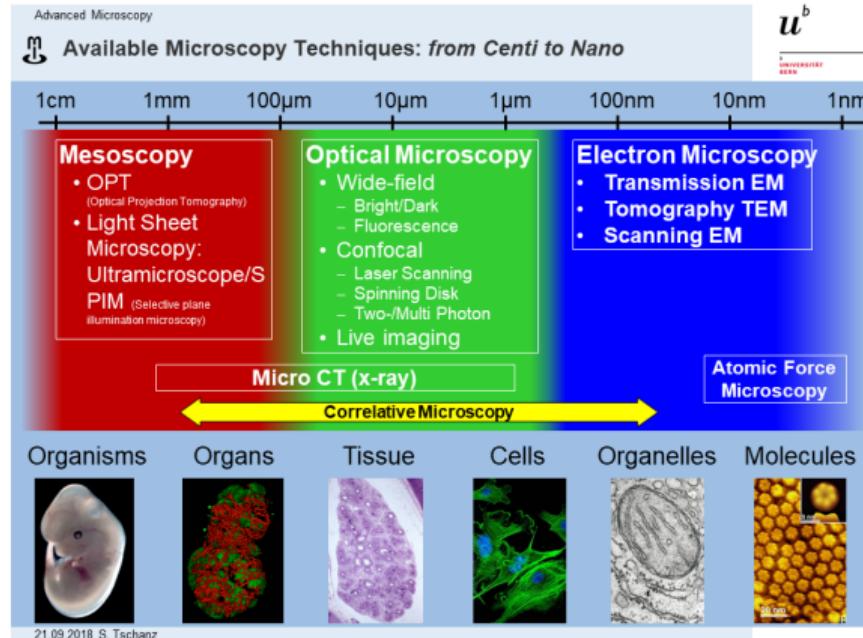

Stefan Tschanz, with permission

Imaging methods

- Light (sheet) microscopy: see lecture of Nadia Mercader Huber
- X-ray imaging
- Electron microscopy
 - *Analytical electron microscopy* by Dimitri
 - *SEM Grundlagen* by Sabine Kässmeyer and Ivana Jaric
 - *Cryoelectron Microscopy & Serial Block Face SEM* by Ioan

u^b

CT-Scanner




youtu.be/2CWpZKuy-NE

u^b

CT History


- 1895: Wilhelm Conrad Röntgen discovers X-rays

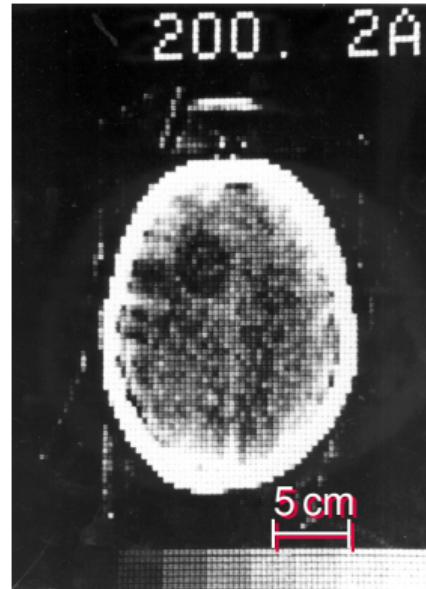

From [15], Figure 5

CT History


- 1895: Wilhelm Conrad Röntgen discovers X-rays
- Cormack used a collimated ^{60}Co source and a Geiger counter as a detector [12]
- 1976: Hounsfield worked on first clinical scanner [13]

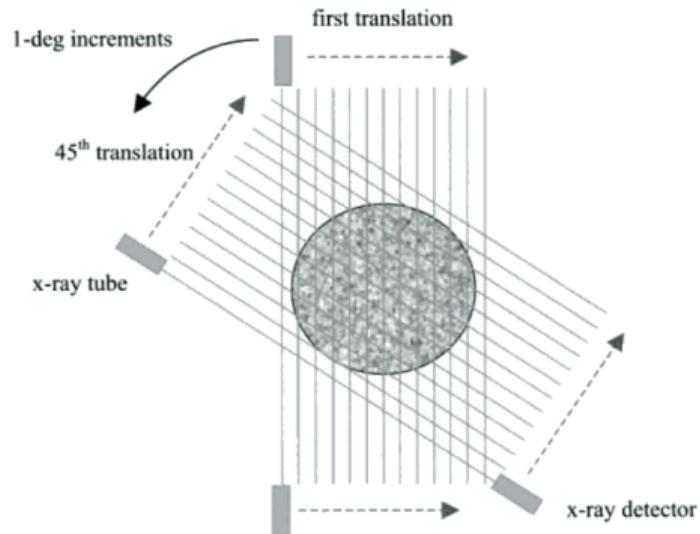

From [14], Figure 1.12

CT History


- 1895: Wilhelm Conrad Röntgen discovers X-rays
- Cormack used a collimated ^{60}Co source and a Geiger counter as a detector [12]
- 1976: Hounsfield worked on first clinical scanner [13]
- CT scanner generations
 - First generation

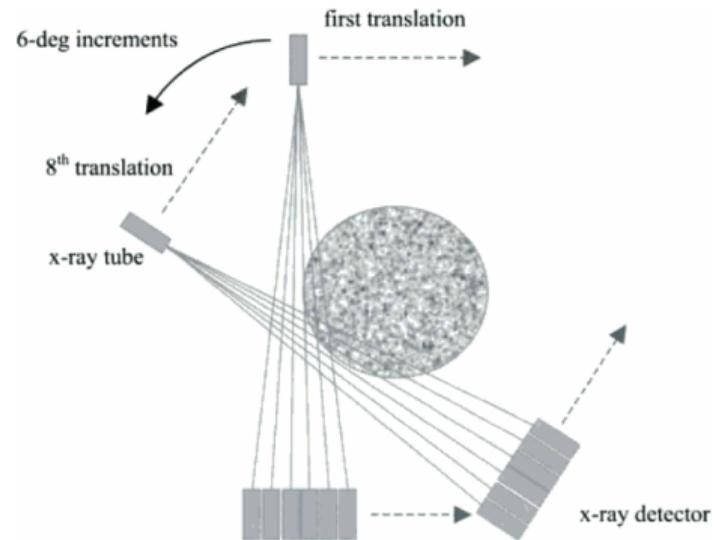

From [14], Figure 1.13

CT History

- 1895: Wilhelm Conrad Röntgen discovers X-rays
- Cormack used a collimated ^{60}Co source and a Geiger counter as a detector [12]
- 1976: Hounsfield worked on first clinical scanner [13]
- CT scanner generations
 - First generation
 - Second generation

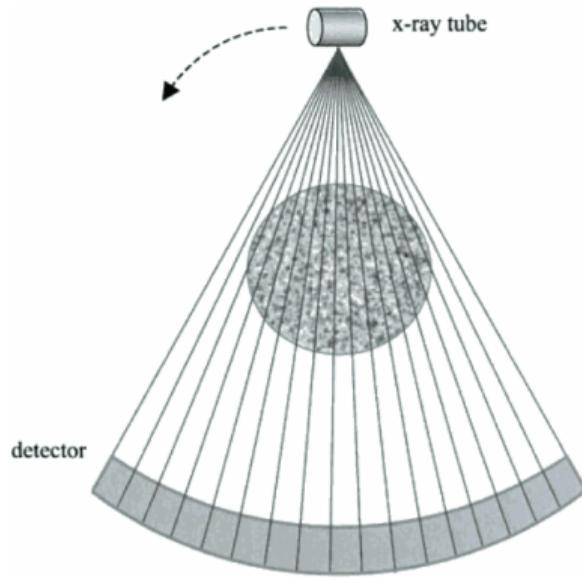

From [14], Figure 1.14

CT History

- 1895: Wilhelm Conrad Röntgen discovers X-rays
- Cormack used a collimated ^{60}Co source and a Geiger counter as a detector [12]
- 1976: Hounsfield worked on first clinical scanner [13]
- CT scanner generations
 - First generation
 - Second generation
 - Third generation

μ CT History I

- X-ray computed tomography began to replace analog focal plane tomography in the early 1970s [16]
- μ CT was first reported in the 1980s, for scanning gemstones
- Lee Feldkamp [17] developed one of the early laboratory microCT systems by assembling a micro-focus cone beam x-ray source, specimen holder and stages, and an image intensifier at Ford Motor Company's Scientific Research Laboratory to nondestructively detect damage in ceramic manufactured automobile parts
- Met with scientists at Henry Ford Hospital and University of Michigan interested in understanding the relationship between the microstructure and biomechanical function of trabecular bone to study osteoporotic fractures [18]
- CT scanners in medical diagnostics, beginning in the early 1970s
- Non-medical use in the late 1970s, for detection of internal defects in fabricated parts and equipment

μ CT History II

- Today: Nondestructive imaging for quantifying the microstructure of organic materials, particularly mineralized bone tissue and the relationships between the mechanical behavior of bone to its structural and compositional properties
- Since the 1990s, μ CT includes imaging of soft tissues and vasculature using radio-opaque contrast agents
- \approx 2500 μ CT systems are in use worldwide with over 1000 publications annually

X-ray interaction

- “X-rays interact with tissue in 2 main ways: photoelectric effect and Compton scatter. To a first approximation, the photoelectric effect contributes to contrast while the Compton effect contributes to noise. Both contribute to dose.” ([19])
 - Photoelectric absorption (τ) is strongly dependent on the atomic number Z of the absorbing material: $\tau \propto \frac{Z^4}{E^{3.5}}$
 - Compton scattering is one of the principle forms of photon interaction and is directly proportional to the (electron & physical) density of the material. It does *not* depend on the atomic number: $\lambda' - \lambda = \frac{h}{m_e c} (1 - \cos \theta)$
- Lowering x-ray energy increases contrast
- X-ray penetration decreases exponentially with sample thickness [20, i. e. Beer-Lambers law]: $I(t) = I_0 e^{-\alpha z}$


Composition of biological tissues

Tissue: content by mass percentage


Element Atomic number	H 1	C 6	N 7	O 8	Na 11	P 15	S 16	Cl 17	K 19	Ca 20
Fat	11.4	59.8	0.7	27.8	0.1		0.1	0.1		
Water	11.2			88.8						
Blood	10.2	11	3.3	74.5	0.1	0.1	0.2	0.3	0.2	
Liver	10.2	13.9	3	71.6	0.3	0.2	0.3	0.2	0.3	
Brain	10.7	14.5	2.2	71.2	0.2	0.4	0.2	0.3	0.3	
Bone	3.4	15.5	4.2	43.5	0.1	10.3	0.3			22.5

u^b

Why μ CT?

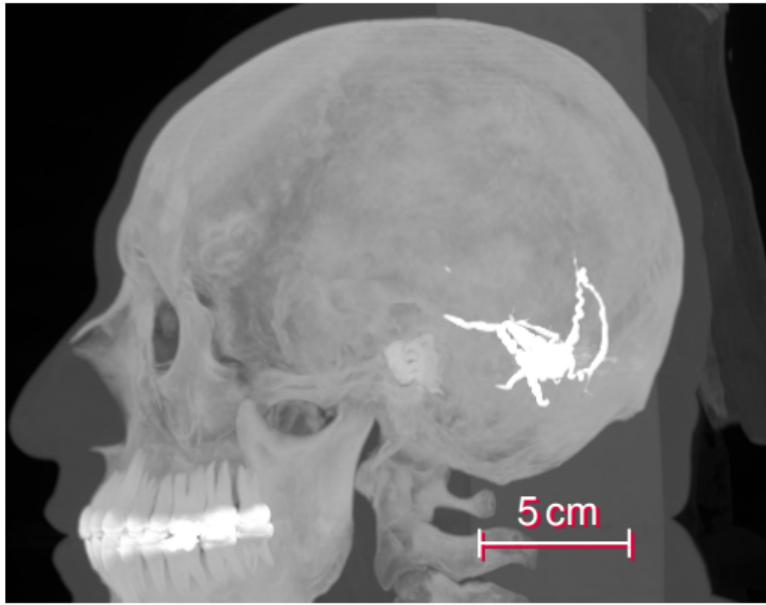


From [21], Subject C3L-02465

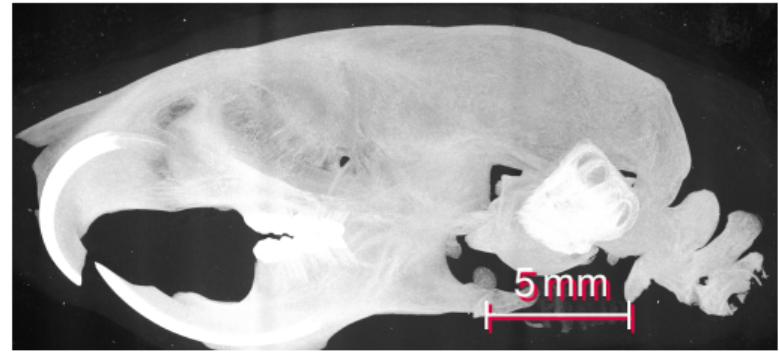

u^b

Why μ CT?

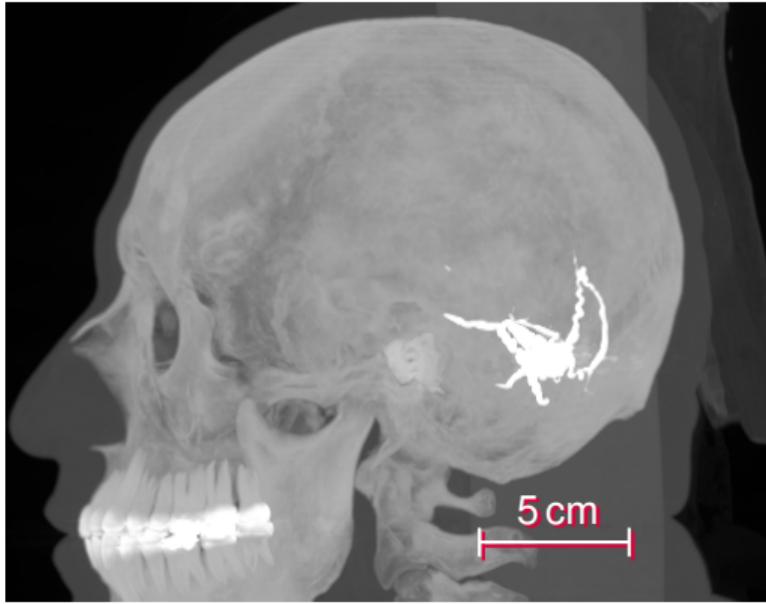


From [21], Subject C3L-02465




u^b

Why μ CT?

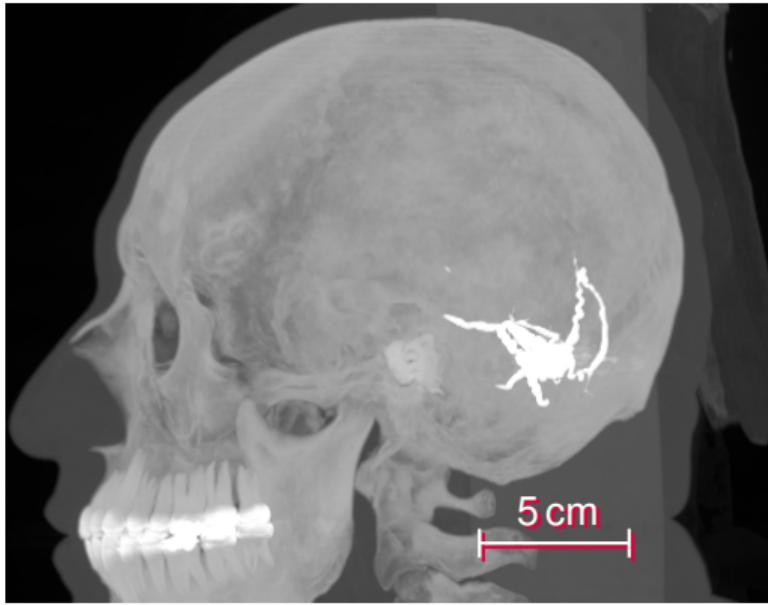


From [21], Subject C3L-02465

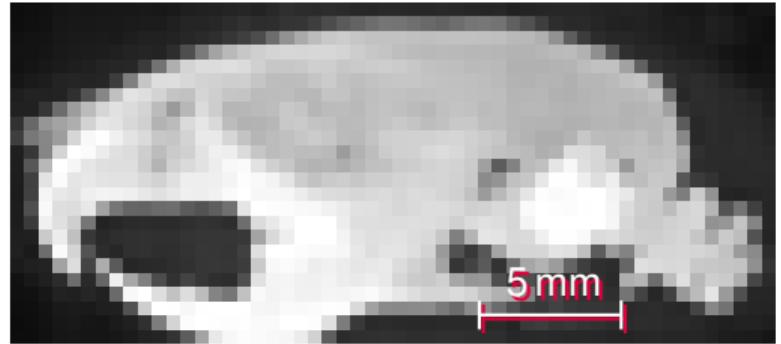


u^b

Why μ CT?

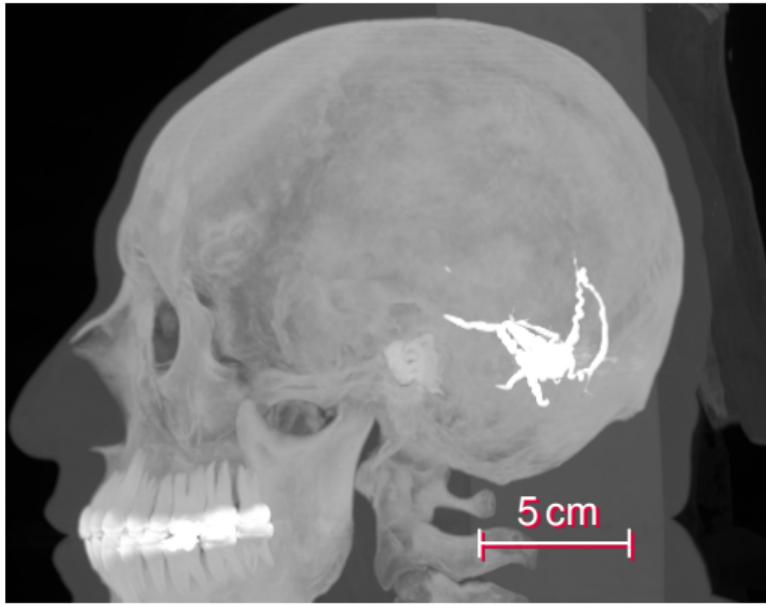


From [21], Subject C3L-02465

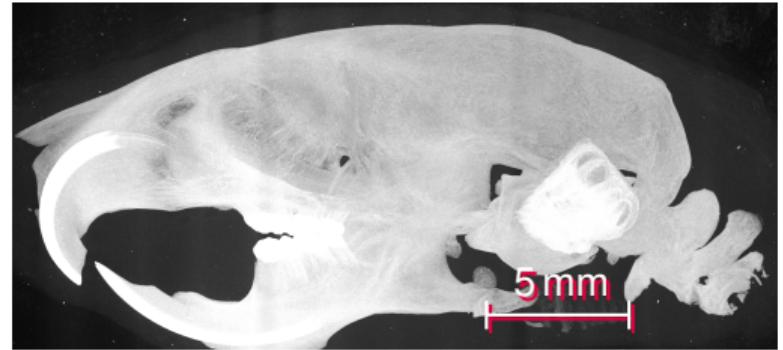


u^b

Why μ CT?






From [21], Subject C3L-02465

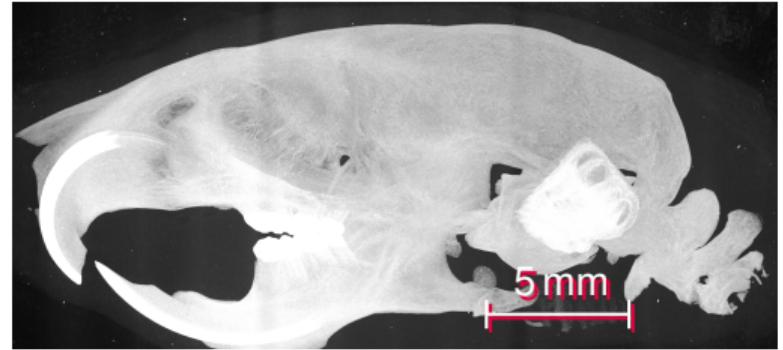

Maximum intensity projection

Projections

Reducing the dimensions of a dataset. For example projecting a volume (3D) to a surface by taking the maximum value across planes for each pixel.

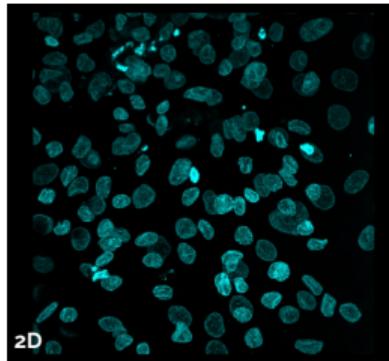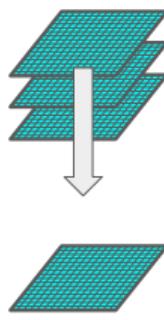

Fundamentals of Digital Image Processing (2022) by Guillaume Witz, Slide 23

u^b

Machinery

- Hospital CT
 - Voxel size around 0.5 mm
- Lab/Desktop CT
 - Voxel size around $7 \mu\text{m}$ (*in vivo*) or $0.5 \mu\text{m}$ (*ex vivo*)
- Synchrotron CT
 - Voxel size down to 160 nm




flic.kr/p/D4rbom

- Hospital CT
 - Voxel size around 0.5 mm
- Lab/Desktop CT
 - Voxel size around 7 μm (*in vivo*) or 0.5 μm (*ex vivo*)
- Synchrotron CT
 - Voxel size down to 160 nm




flic.kr/p/fpTrGu

- Hospital CT
 - Voxel size around 0.5 mm
- Lab/Desktop CT
 - Voxel size around 7 μm (*in vivo*) or 0.5 μm (*ex vivo*)
- Synchrotron CT
 - Voxel size down to 160 nm

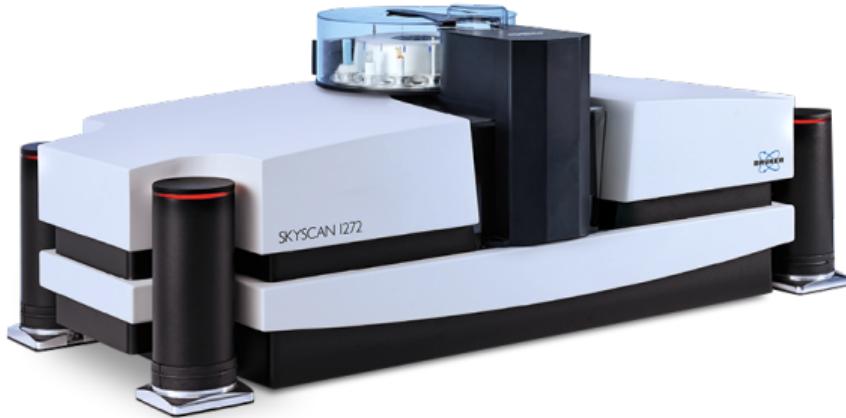

bruker.com/skyscan1272

- Hospital CT
 - Voxel size around 0.5 mm
- Lab/Desktop CT
 - Voxel size around 7 μm (*in vivo*) or 0.5 μm (*ex vivo*)
- Synchrotron CT
 - Voxel size down to 160 nm

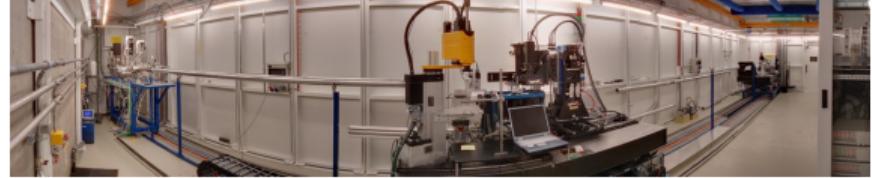


flic.kr/p/7Xhk2Y

u^b

What is happening?

No matter what kind of machine, the basic principle is always the same

- an x-ray source
- a sample
- a detector

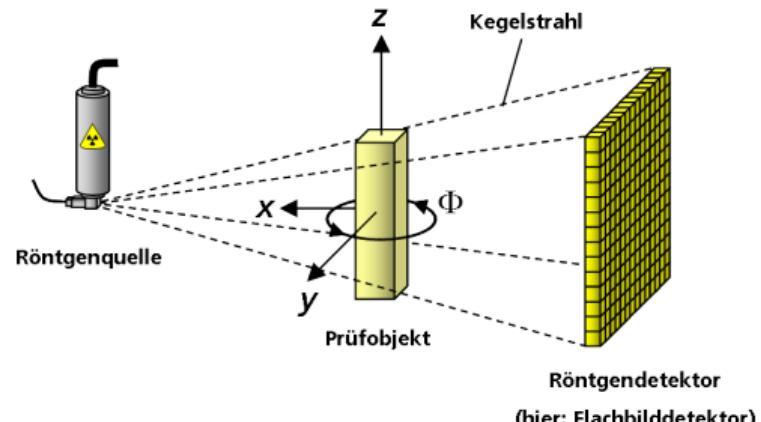


w.wiki/7g3 @①②

u^b

Machinery


u^b

Examples

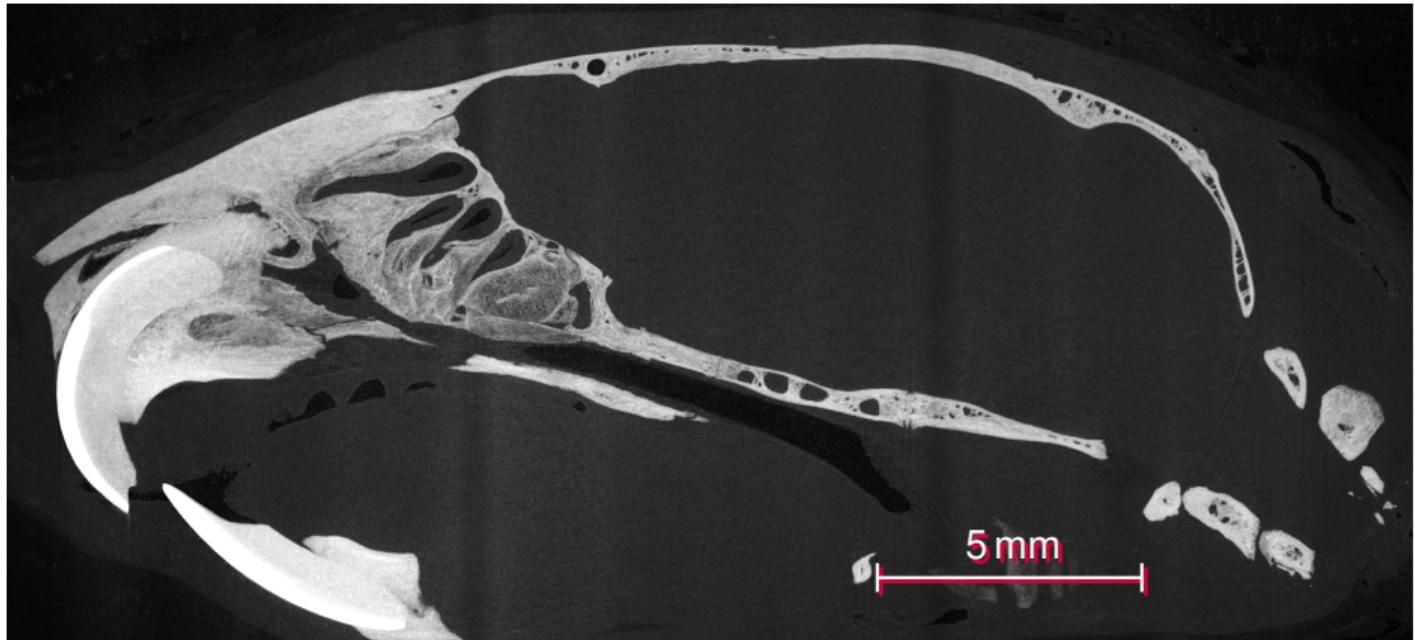


u^b

Examples

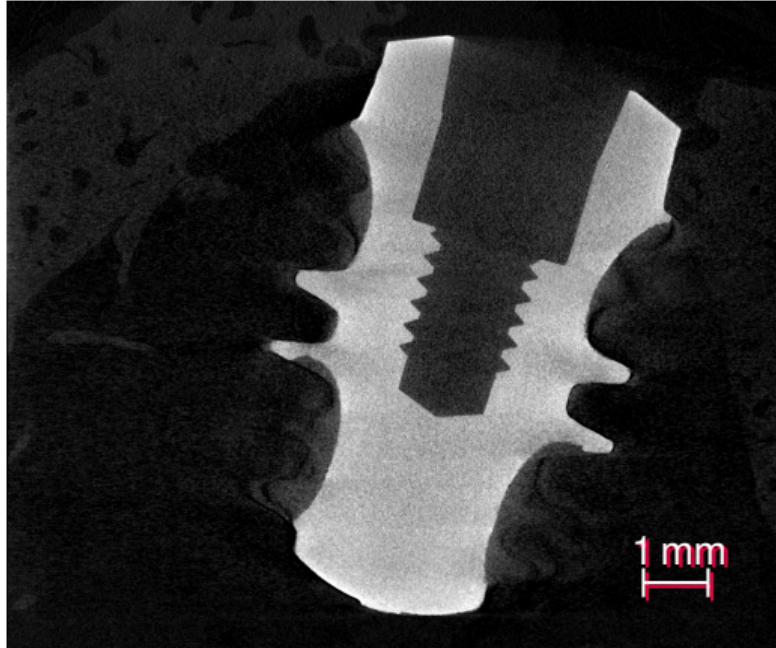

u^b


Examples

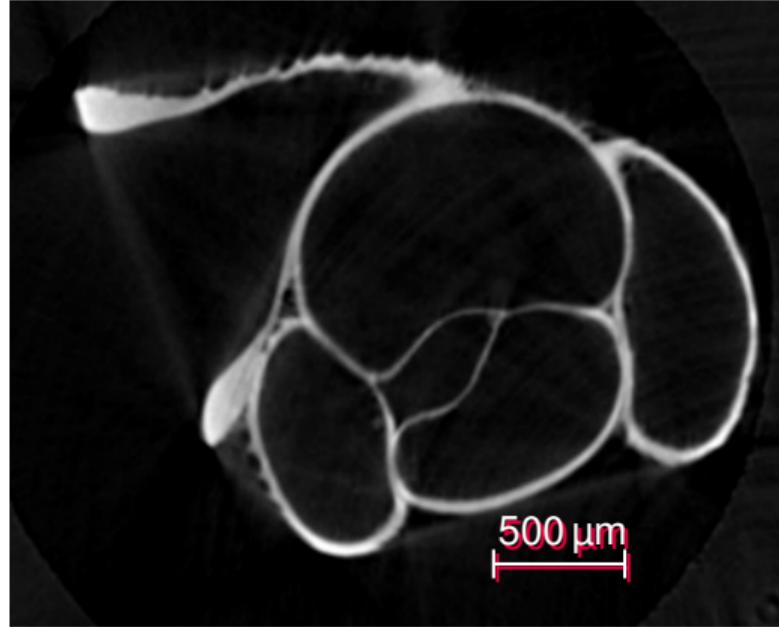

From [8], *Diancta phoenix*

u^b

Examples

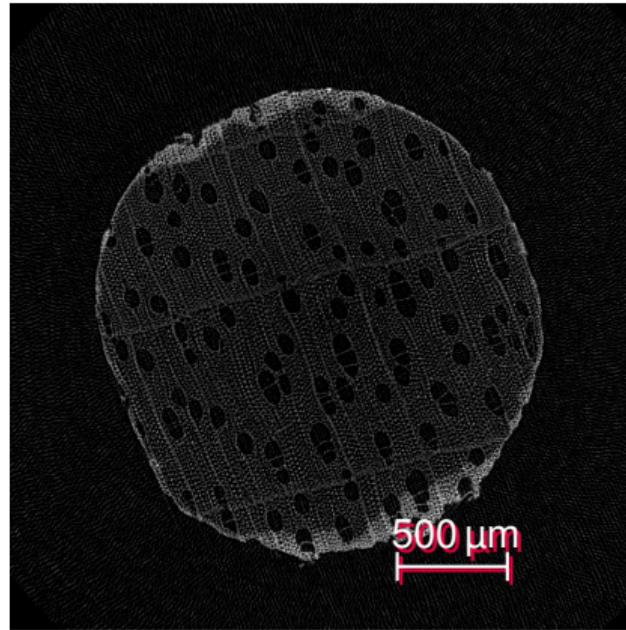

u^b

Examples




u^b

Preparation

- Study design
- Sample preparation

Projections


X-ray generation and contrast

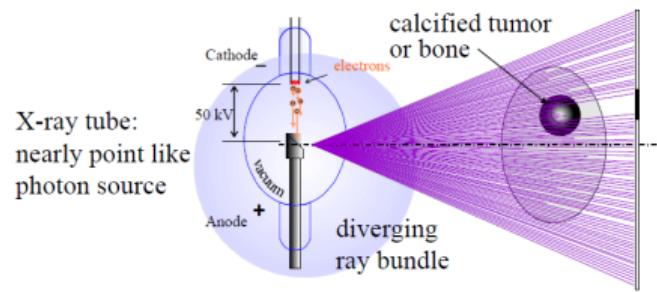

X-ray tube:
nearly point like
photon source


Contrast is given by
absorption of intensity I

Note that contrast is negative
X-ray shadowgraphy
is a bright field technique

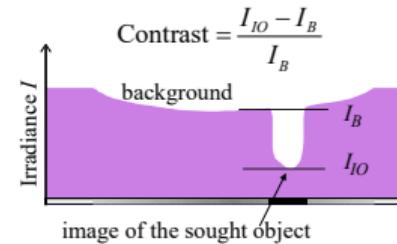


Contrast, Magnification and Resolution—Laws of Physics for Microscopists (1, 2022) by Martin Frenz, Slide 21

u^b Projection acquisition

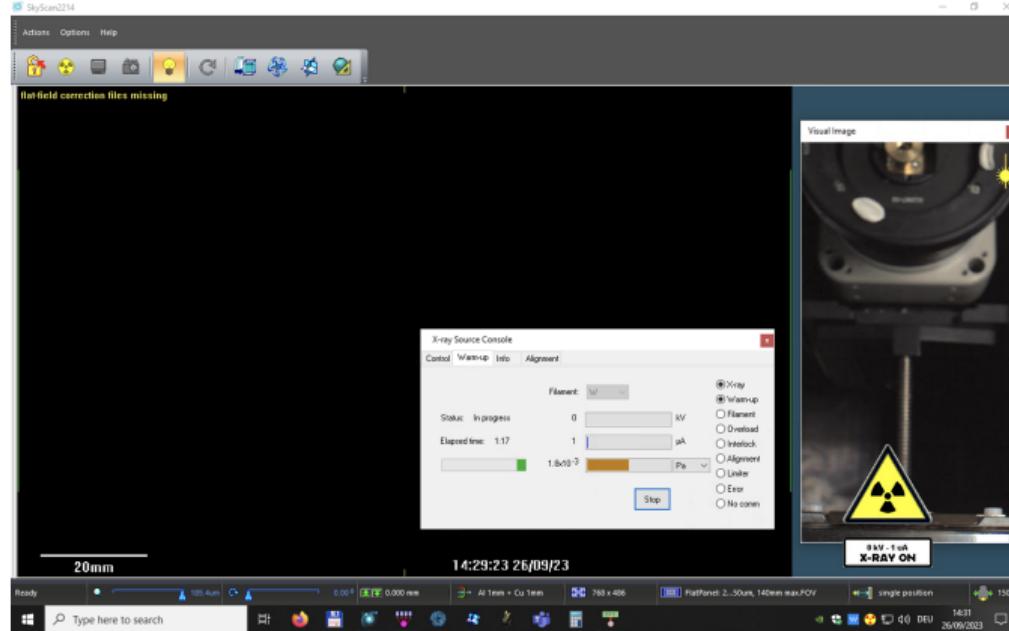

u^b

Projections

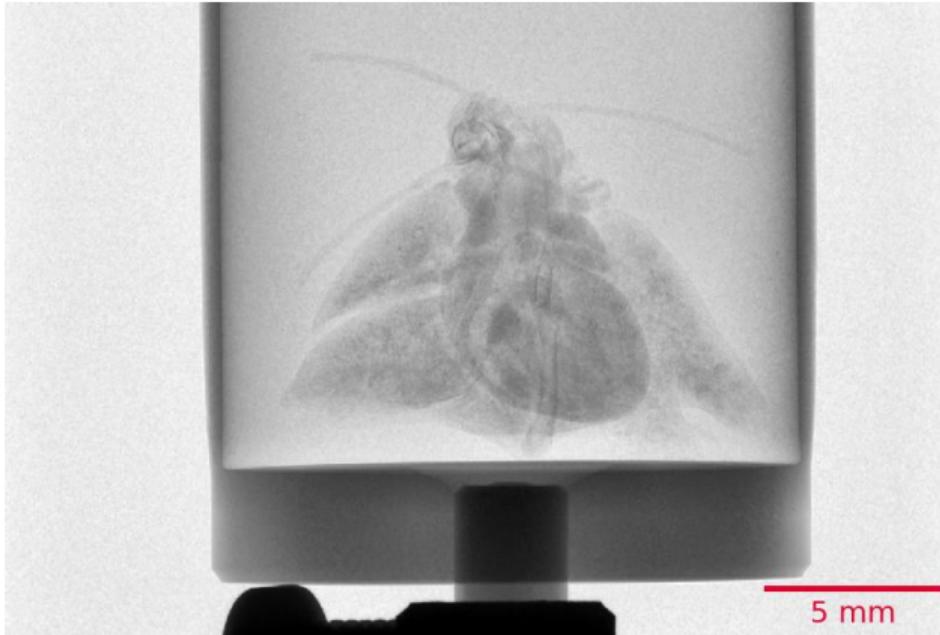


Projections

- A (micro-focus) x-ray source illuminates the object
- The x-rays penetrate the sample and are attenuated
- A scintillator converts the x-rays to visible light
- A (planar) x-ray detector collects (magnified) projection images.
- The projections are recorded on disk


u^b

Reconstructions

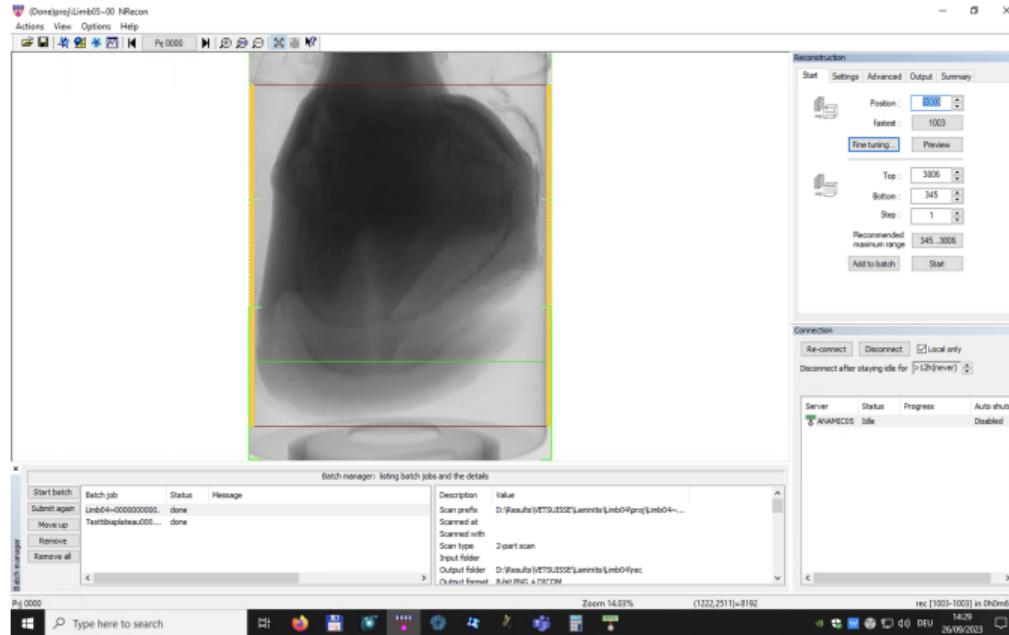


u^b

Reconstructions

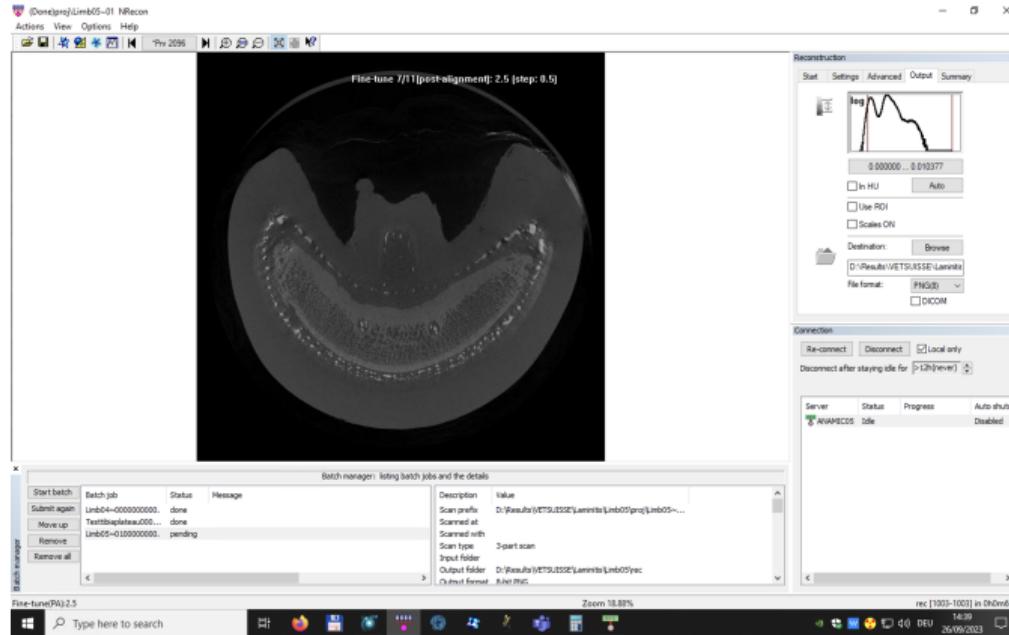

u^b

Reconstructions

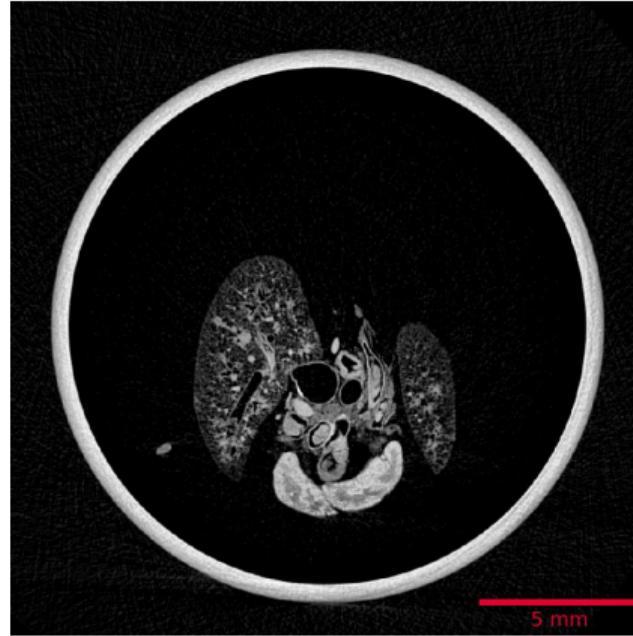

Reconstructions

- Based on hundreds of angular views acquired while the object rotates, a computer synthesizes a stack of virtual cross section slices through the object.
- Radon Transformation
- Filtered back projection
- Fan beam reconstruction
- Corrections (beam hardening, etc.)
- Writing to stack

u^b

Visualization



- Based the on reconstructions, a computer synthesizes a three-dimensional view of the scanned sample

u^b

What to use?

- ImageJ/Fiji [22]
- Also see *Fundamentals of Digital Image Processing* by Guillaume Witz
- Reproducible research
 -  in Jupyter [23]
 - **git**
 - Script all your things!
 - Data repositories; i. e. sharing is caring!


Quantitative data

- Pretty images are nice, but we need quantitative numbers
- Segmentation
- Characterization

Internal morphology of human teeth

Collaboration with zmk bern – Zahnmedizinische Kliniken

- Numbers instead of just pretty images
- Segments
- Labels

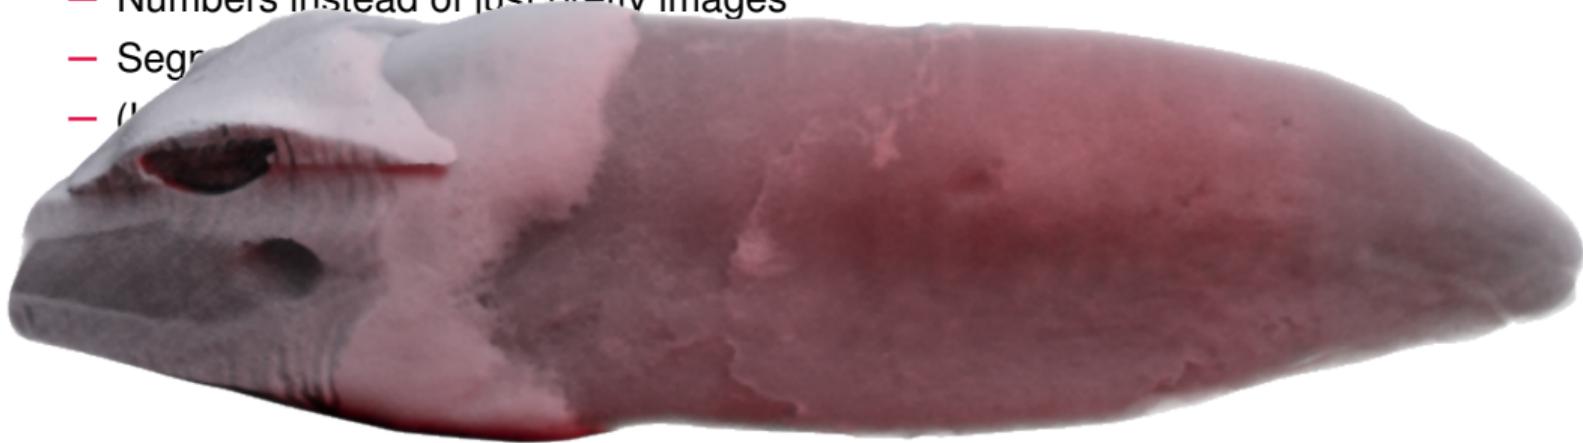

Internal morphology of human teeth


Collaboration with zmk bern – Zahnmedizinische Kliniken

- Numbers instead of just pretty images
- Segmentation of teeth and root canal
- (Unbiased) Characterization
- Reproducible and automated image analysis ( in Jupyter [23])
- Two publications:
 - [10], BMC Oral Health, doi.org/gjpw2d
 - [24], Scientific Reports, doi.org/g7r8

- 104 extracted human permanent mandibular canines
- μ CT imaging
- Root canal configuration, according to Briseño-Marroquín *et al.* [25]
- *Reproducible* analysis [26], e. g. you can click a button to double-check or recalculate the results yourself!



- 104 extracted human permanent mandibular canines
- μ CT imaging
- Root canal configuration, according to Briseño-Marroquín *et al.* [25]
- *Reproducible* analysis [26], e. g. you can click a button to double-check or recalculate the results yourself!

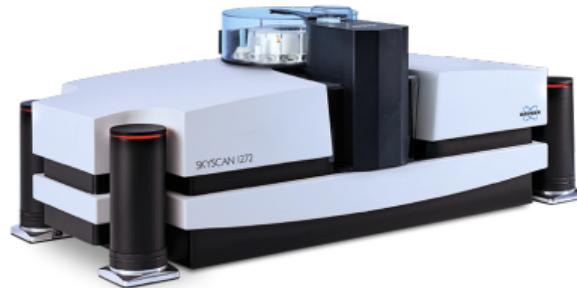

[bruker.com/sky\(scan\)1272](http://bruker.com/sky(scan)1272)

- 104 extracted human permanent mandibular canines
- µCT imaging
- Root canal configuration, according to Briseño-Marroquín *et al.* [25]
- *Reproducible* analysis [26], e. g. you can click a button to double-check or recalculate the results yourself!


```
Scanner=SkyScan1272
Instrument S/N=15G09089-B
Software Version=1.1.19
Filename Prefix=Tooth045~00
Number Of Files= 482
Number Of Rows= 1092
Number Of Columns= 1632
Source Voltage (kV)= 80
Source Current (uA)= 125
Image Pixel Size (um)=9.999986
Exposure (ms)=950
Rotation Step (deg)=0.400
Frame Averaging=ON (3)
Filter=Al 1mm
Study Date and Time=02 Jul 2020 08h:23m:34s
Scan duration=0h:39m:51s
```

- 104 extracted human permanent mandibular canines
- μ CT imaging
- Root canal configuration, according to Briseño-Marroquín *et al.* [25]
- *Reproducible* analysis [26], e. g. you can click a button to double-check or recalculate the results yourself!

Sample changer on the SkyScan 1272
In total:


- 13 days of *continuous* μ CT scanning
- 819 GB of raw data
- 230 648 TIFF projections
- 326 GB data as input for analysis
- 282 062 PNG reconstructions

- 104 extracted human permanent mandibular canines
- μ CT imaging
- Root canal configuration, according to Briseño-Marroquín *et al.* [25]
- *Reproducible* analysis [26], e. g. you can click a button to double-check or recalculate the results yourself!

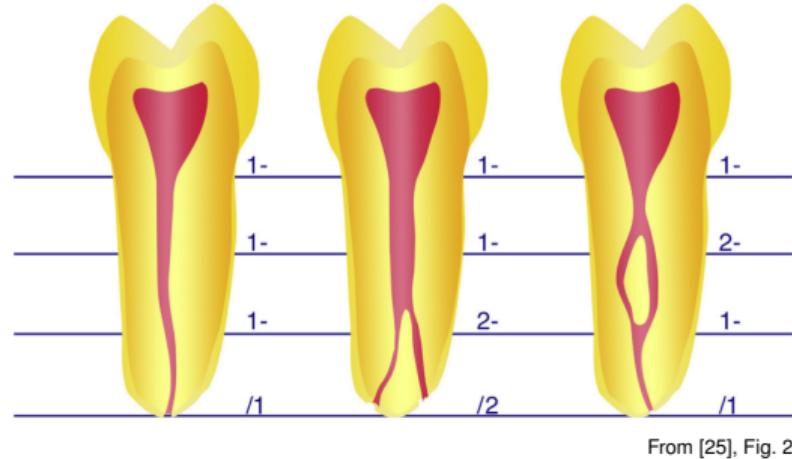

From [25], Fig. 2

- 104 extracted human permanent mandibular canines
- μ CT imaging
- Root canal configuration, according to Briseño-Marroquín *et al.* [25]
- *Reproducible* analysis [26], e. g. you can click a button to double-check or recalculate the results yourself!

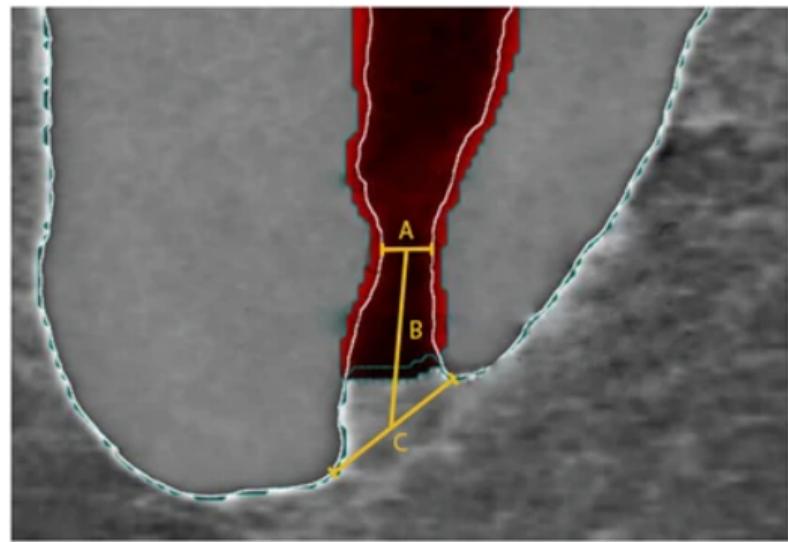

From [27], Fig. 1

- 104 extracted human permanent mandibular canines
- μ CT imaging
- Root canal configuration, according to Briseño-Marroquín *et al.* [25]
- *Reproducible* analysis [26], e. g. you can click a button to double-check or recalculate the results yourself!



gph.is/2nqkple

u^b

How?

- 104 extracted human permanent mandibular canines
- µCT imaging
- Root canal configuration, according to Briseño-Marroquín *et al.* [25]
- *Reproducible* analysis [26], e. g. you can click a button to double-check or recalculate the results yourself!

The screenshot shows a GitHub repository interface. At the top, there are buttons for 'master', '1 branch', '1 tag', 'Go to file', 'Add file', and 'Code'. Below this is a list of commits from user 'habli' with the message 'Update actions file'. The commits are:

File	Message	Time Ago
.github/workflows	Update actions file	20 days ago
.gitignore	Only 'mode' changes	2 months ago
DownloadFromOSF.ipynb	Clean run of download script	22 days ago
README.md	Typo in Binder badge & link to full repo on Binder	22 days ago
Tooth.Border.jpg	Only 'mode' changes	2 months ago
Tooth.Characterization.jpg	Only 'mode' changes	2 months ago
ToothAnalysis.ipynb	Only select a subset if we actually have data.wq	22 days ago
ToothAxisSize.ipynb	Clean run of notebook	22 days ago
ToothDisplay.ipynb	Display Tooth045 for manuscript	22 days ago
requirements.txt	We also need this	2 months ago
treebeard.yaml	Add treebeard configuration	20 days ago

Below the commits is a 'README.md' file with the following content:

```
README.md
[![DOI](https://zenodo.3999402/treebeard.yaml)](https://zenodo.3999402/treebeard.yaml) [![Funding](https://zenodo.3999402/funding.svg)](https://zenodo.3999402/funding.svg)
[![Launch Binder](https://zenodo.3999402/binder-launch.svg)](https://zenodo.3999402/binder-launch.svg)


A big tooth cohort

We scanned a big bunch of teeth for a team of the dental clinic of the University of Bern.

To get an overview of the samples while we scanned the whole tooth cohort we generated a preview and analysis notebook. The analysis notebook (with download possibility for two of the >100 teeth) can be started in your browser by clicking on the 'Binder' badge above, without installation of any software. If you'd like to start a Binder instance with the full repository, you can click here.
```

μ ^b




μ CT imaging

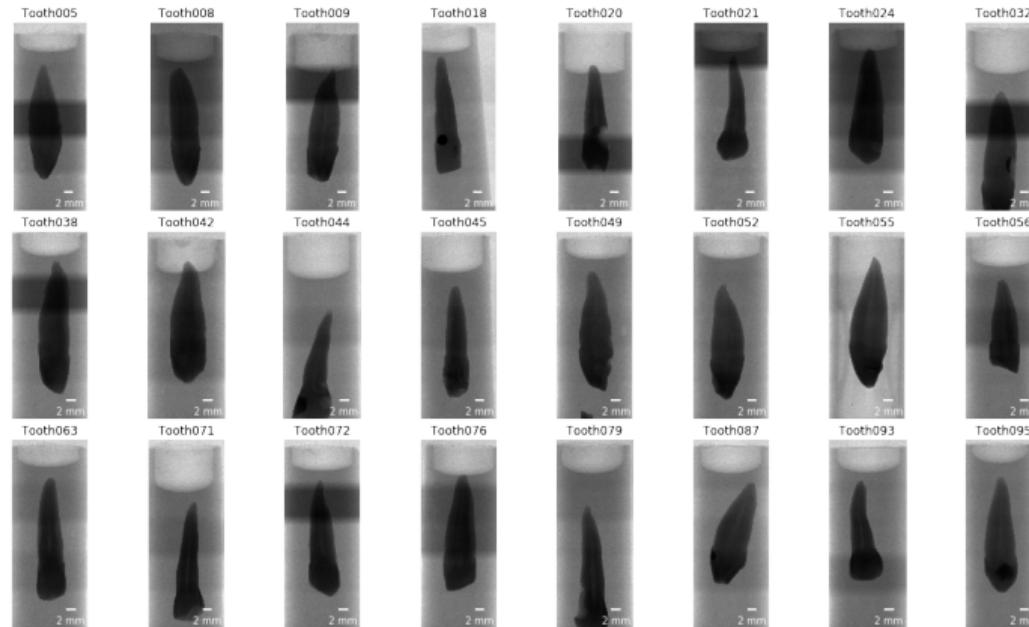

u^b

Dataset cropping




- Full datasets: 326 GB
- Cropped datasets: 115 GB

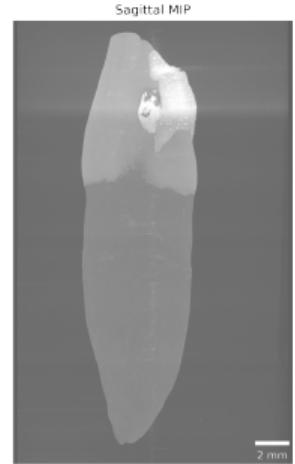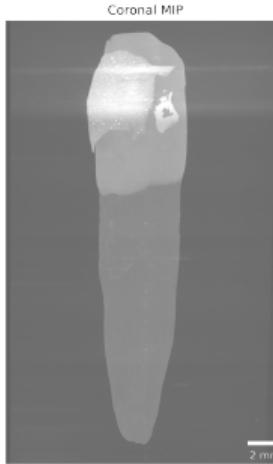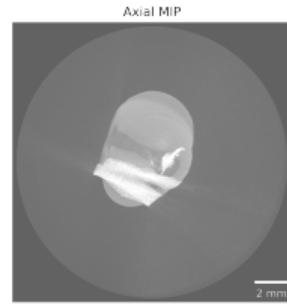

u^b

Dataset cropping

- Full datasets: 326 GB
- Cropped datasets: 115 GB

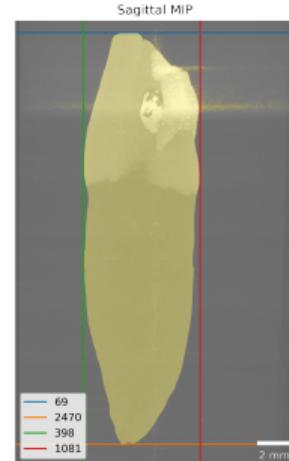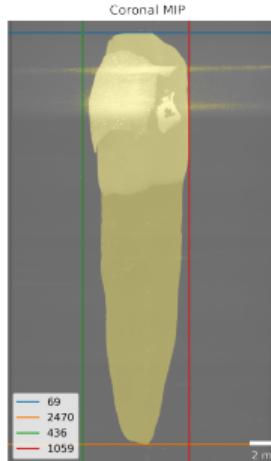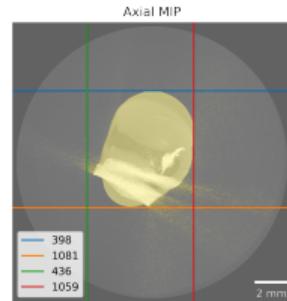


u^b

Tooth morphology



u^b


Tooth morphology

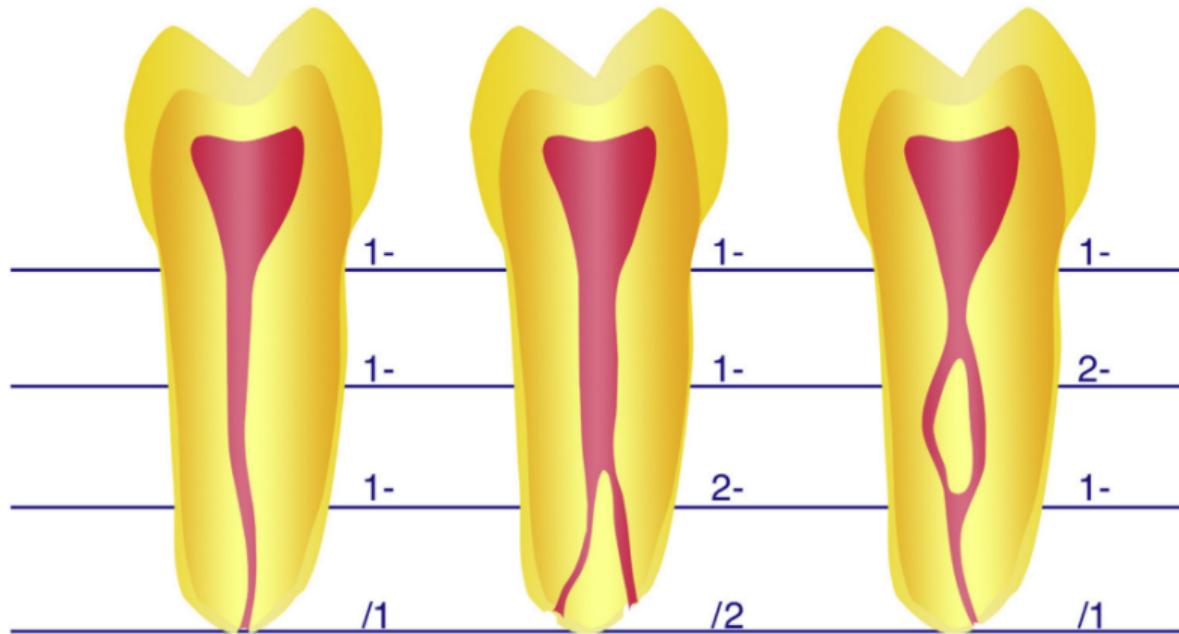

From [25], Fig. 2


u^b

Tooth morphology

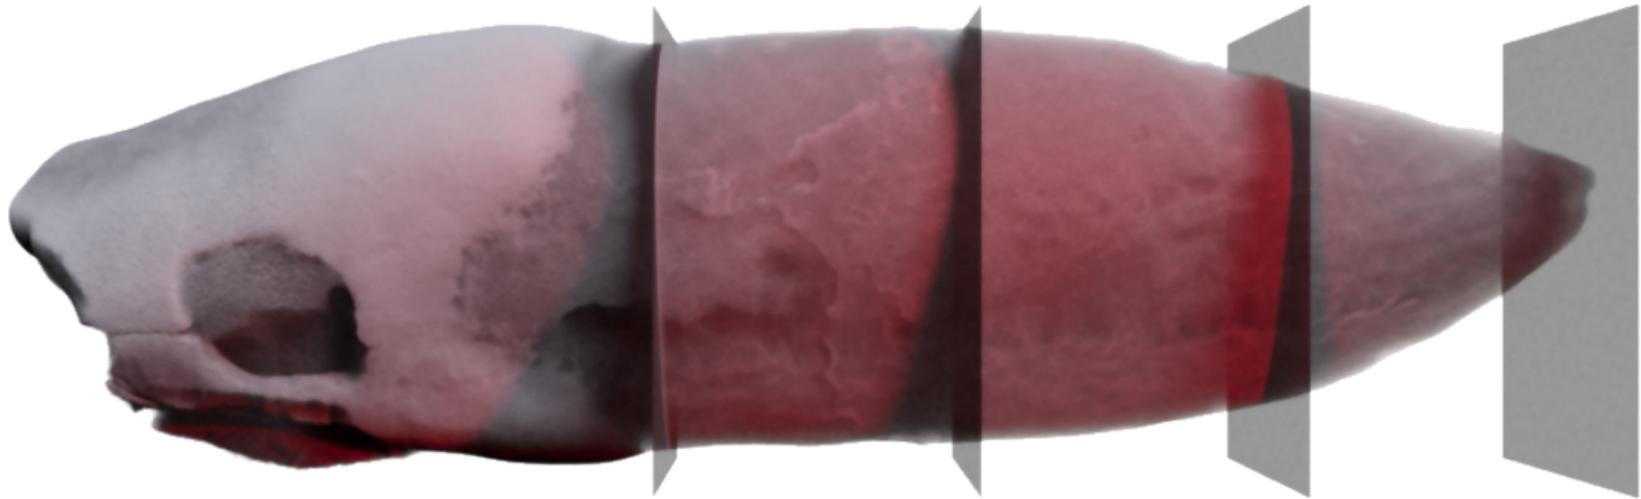


u^b

Detection of enamel-dentin border

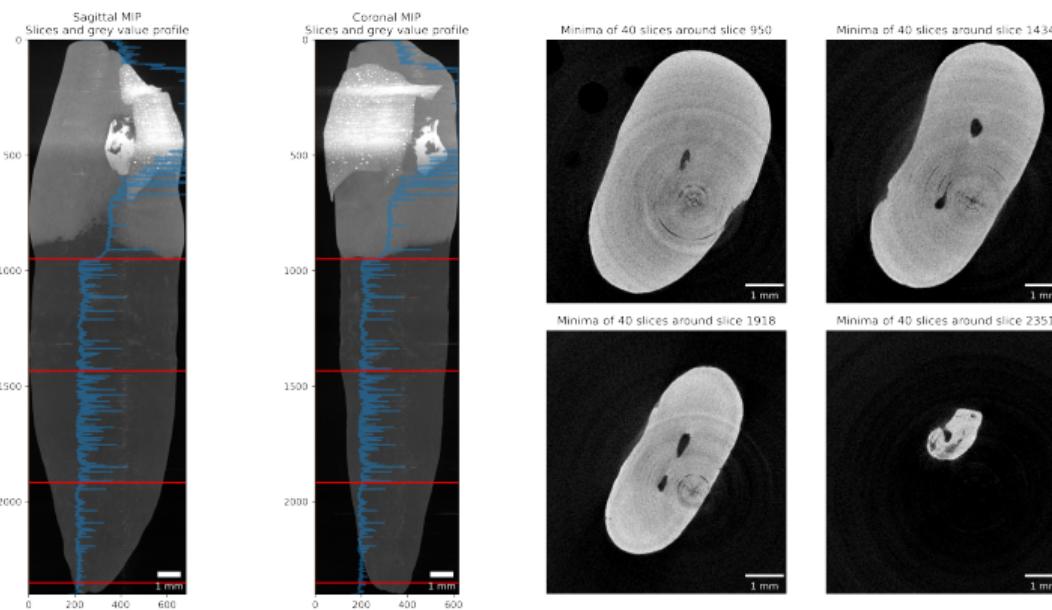

u^b

Detection of enamel-dentin border

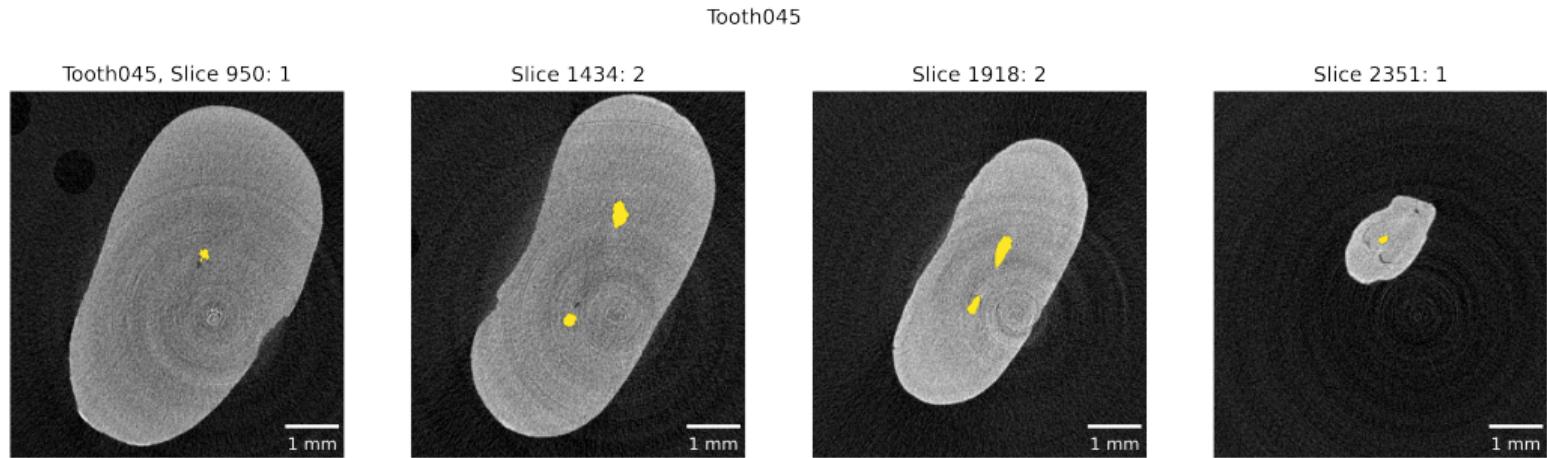


u^b

Outcome root canal configuration classification

Roots	RCC	#	%	
Single (N=98)	1-1-1/1	73	74.5	
	1-1-1/2	14	14.3	
	1-1-1/3	1	1.0	
	1-1-1/4	2	2.1	
	1-1-2/1	1	1.0	
	1-2-1/1	4	4.1	
	1-2-1/2	1	1.0	
	1-2-2/2	1	1.0	
	2-3-1/1	1	1.0	
Double (N=3)	Buccal	1-1-1/1	2	66.6
		1-2-1/1	1	33.3
	Lingual	1-1-1/1	2	66.6
		1-1-1/2	1	33.3


u^b

Extraction of root canal space

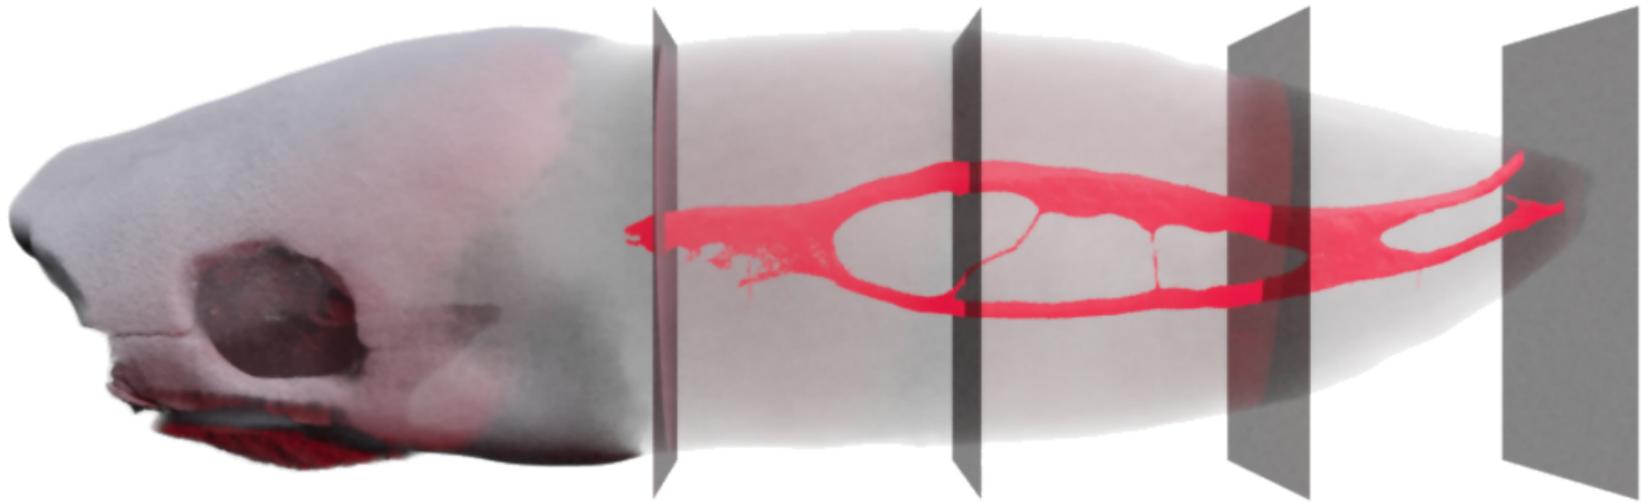


u^b

Results of root canal space extraction

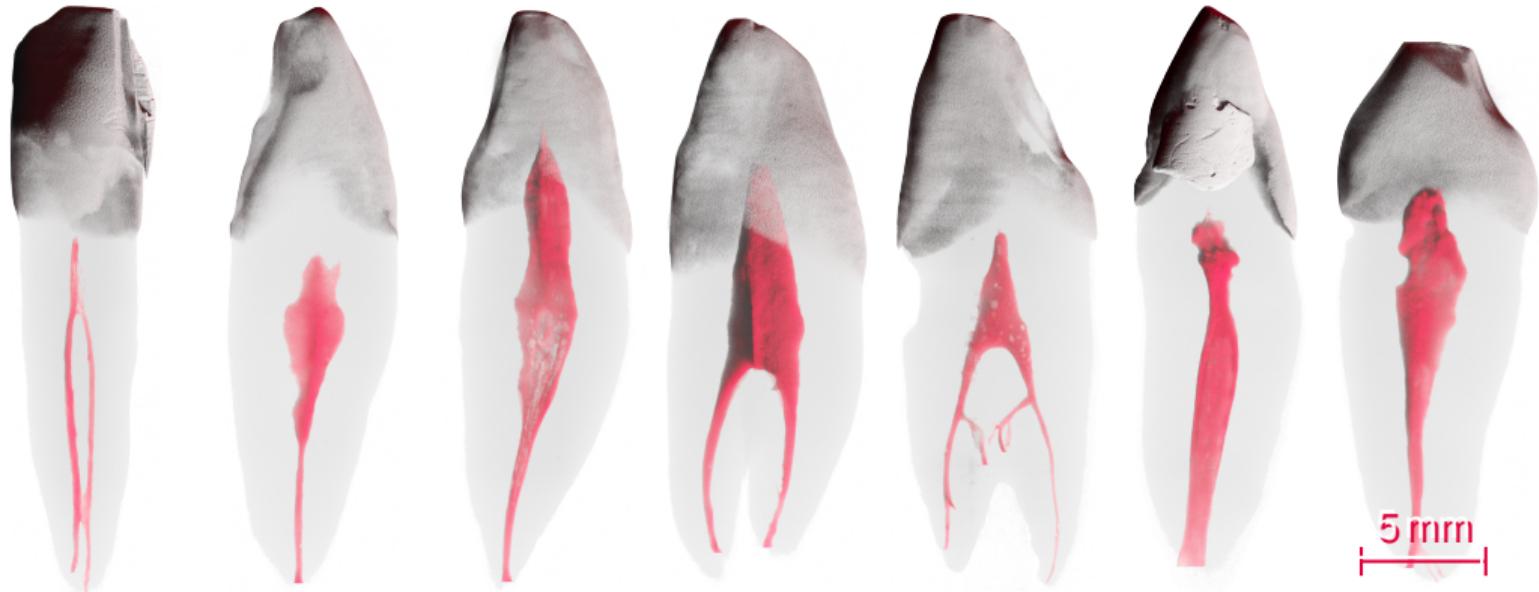

u^b


Analysis of the physiological foramen geometry

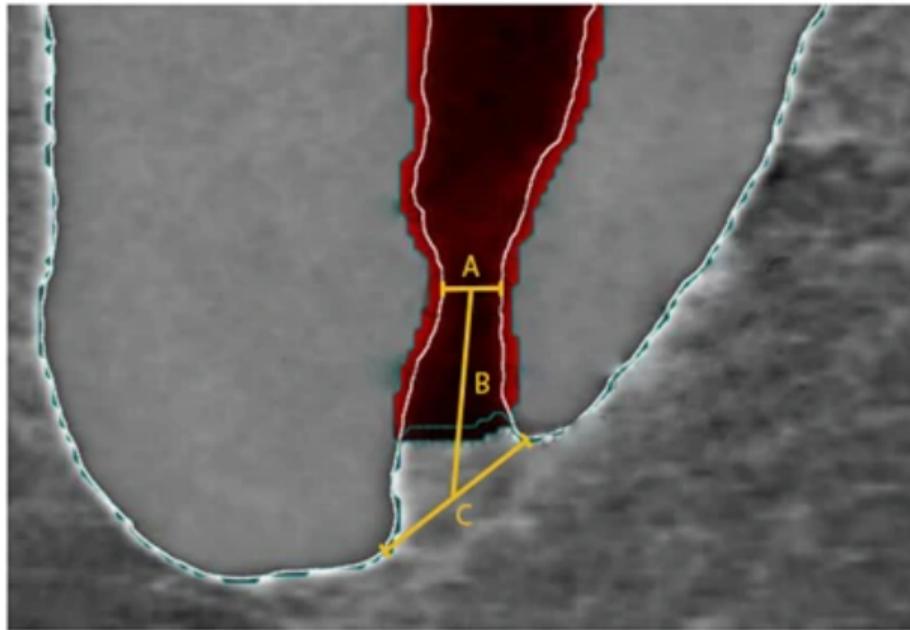

From [27], Fig. 1

u^b

Analysis of the physiological foramen geometry

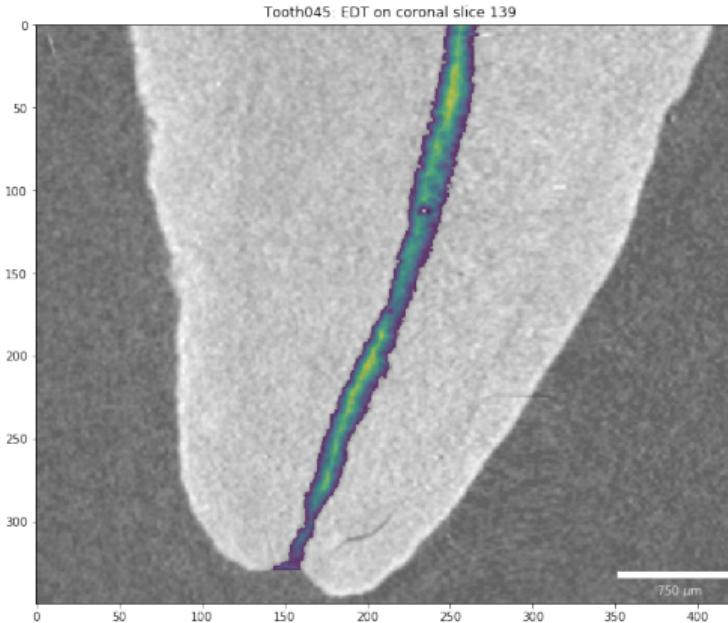


Conclusion ZMK

- Efficient use of time, e. g. more teeth does not mean more (human) work
- Reproducible analysis with *free and open-source* software, usable by *anyone*
- Objective analysis, e. g. no operator bias

u^b

Metal foam

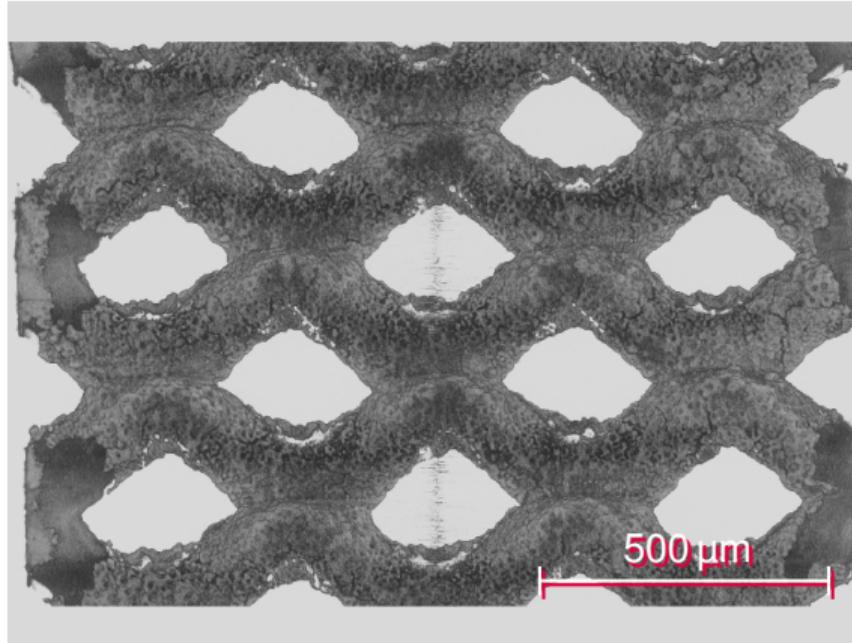


Etienne Berner NanoElectroCatalysis Group

u^b

Data wrangling by example: Cichlids

Collaboration with team of *Aquatic Ecology & Evolution*, from the Institute of Ecology and Evolution [11]


- 133 Cichlids from Lake Victoria, East Africa
 - Functional anatomy of the skulls and jaws
 - 6–18 cm in size
- 375 scans in total
 - Voxelsizes from 3.5–50 µm
 - 46 days of scanning time
 - 9.8 TB of raw data
 - 1.5 TB/+1 000 000 reconstructions

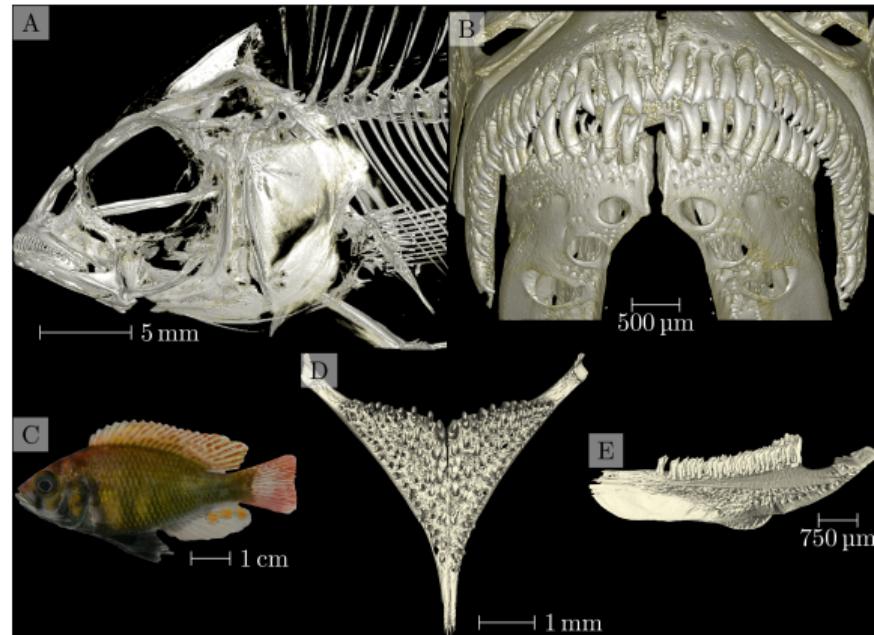

[11] D. Haberthür *et al.*, DOI: gsst8t.






u^b

Cichlids

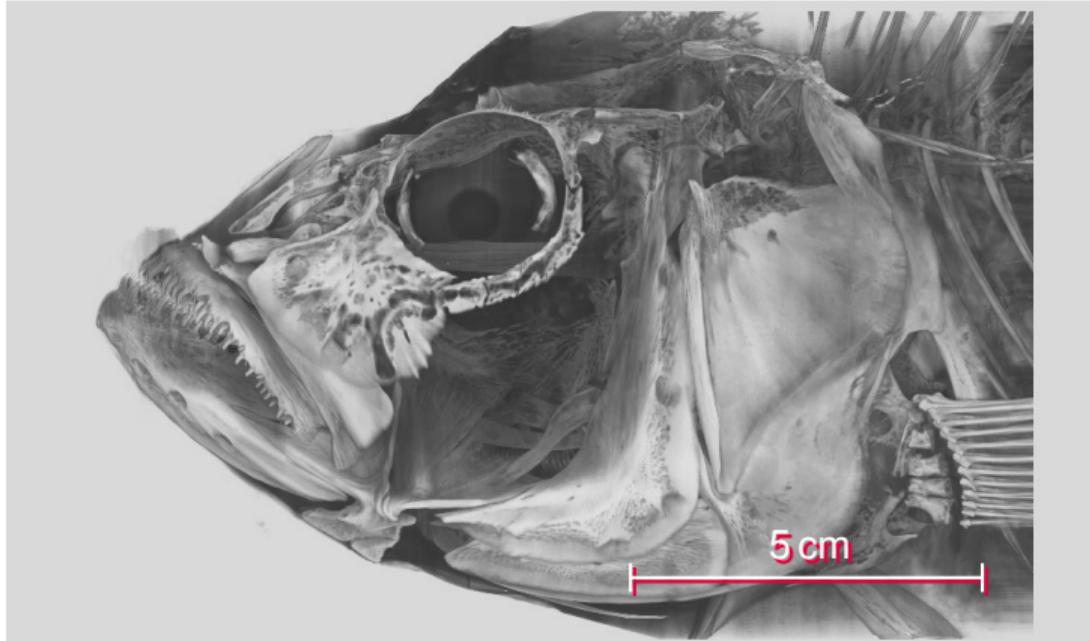

u^b

Data wrangling by example: Cichlids



3D view

u^b

Thanks!

- Thanks for listening to me!
- What questions do you have for me?

Colophon

- This BEAMER presentation was crafted in \LaTeX with the (slightly adapted) template from *Corporate Design und Vorlagen* of the University of Bern.
 - Complete source code: git.io/fjpP7
 - The \LaTeX code is automatically compiled with a GitHub action to a (handout) PDF which you can access here: git.io/JeQxO
- Did you spot an error?
 - File an issue: git.io/fjpPb
 - Submit a pull request: git.io/fjpPN
 - Send me an email: david.haberthuer@unibe.ch