

## PEMANTAPAN MUTU INTRA LABORATORIUM BIDANG KIMIA KLINIK RUMAH SAKIT " DHARMA NUGRAHA "

JI. Balai Pustaka Baru No. 19 Rawamangun - Jakarta Timur, Telepon 021-4707433; Fax 021-4707428

Control Serum :981043		Reagen Cholesterol			Ref :981813		Agu-23	Pemeriksaan	Kolesterol	
Thermo Ind	liko	No.Lot	Nilai Mean	Batas peringatan (x+	-2SD)	1 SD			Metode	Chol - Oxidase
Normal	NORTROL	981043/V884	174	147,9	200,1	8,7		30/06/2025	Satuan	mg/dL
Path	ABTROL	981044/V883	278	236,3	319,7	13,9		30/06/2025	Alat	THERMO INDIKO

*)	Tgl			Petugas
	Hasil	Normal	Patologis	
	1	165	255	Fara
	2	155	250	Agus
	3	158	260	Agus
	4	160	264	Vinna
	5	161	261	Vinna
	6	167	265	Fara
	7	162	272	Fara
	8	170	279	Yanti
	9	174	265	Yanti
	10	160	265	Vinna
	11	162	264	Vinna
	12	157	255	Agus
	13	158	260	Agus
	14	165	266	Yanti
	15	170	270	Yanti
	16	168	270	Vinna
	17	165	278	Vinna
	18	161	268	Fara
	19	168	269	Fara
	20	166	269	Agus
	21	165	271	Agus
	22	165	263	Yanti
	23	170	278	Yanti
	24	165	265	Fara
	25	161	269	Fara
	26	161	267	Agus
	27	162	270	Agus
	28	157	267	Vinna
	29	160	265	Vinna
	30	165	278	Fara
	31	170	280	Fara

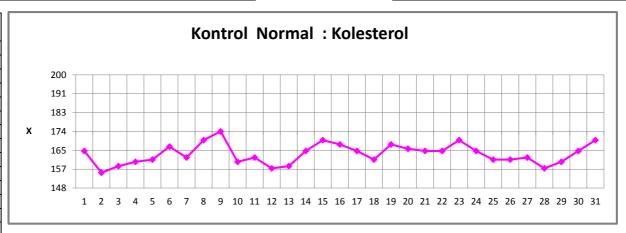

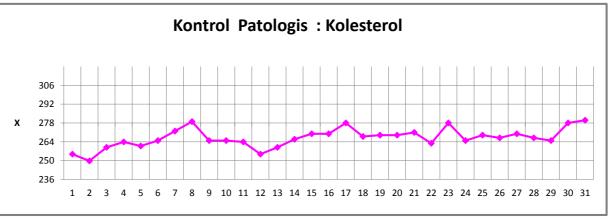

## Kenustakaan

- \* Sun Diagnostics Total Error Limits for variety of Laboratory testdefined by CLIA
- \*\* Westgard JO,Phd; Basic QC Practices 2 nd Edition; 2008; page 33, 195

## CV Maksimum \* ditetapkan

PARAMETER	CV (%)
BIL Total	7
Kolesterol	6
Kreatinin	6
Glukosa	5
Protein Total	3
Albumin	6
Ureum	8
Trigliserida	7
SGOT	7
SGPT	7
Asam Urat	6
Alkali Fosfatase	7
Gamma GT	7
Kolesterol HDL	5,4
Kolesterol LDL	6,3
Calcium	5
Magnesium	10
Natrium	1,5
Kalium	2.7
Chlorida	2
Fosfor	4,3

Aturan Kontrol : Westgard**			
Peringatan	1 <b>-</b> 2S		
Penolakan	1-35		
Penolakan	2 <b>–</b> 2S		
Penolakan	R – 4S		

Diketahui oleh : Koordinator Laboratorium Widya Astuti



Mean	163,65	268,00
SD	4,62	277,00
CV	2,82%	103,36%