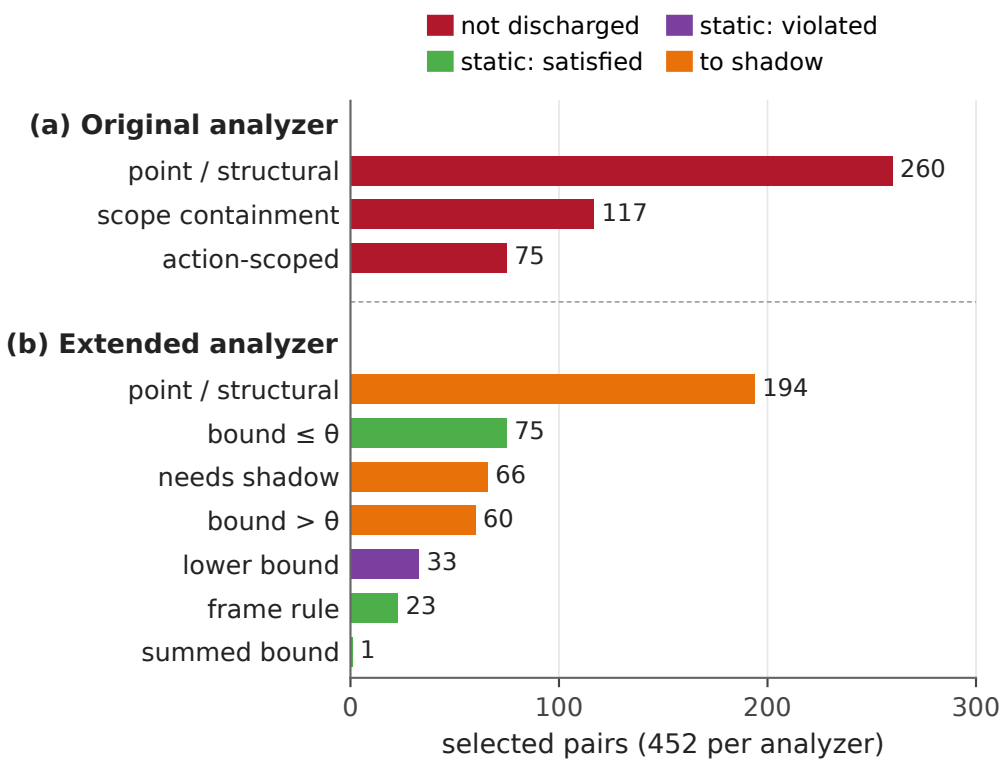
not discharged
static: violated
static: satisfied
to shadow
(a) Original analyzer
point / structural
260
scope containment
117
action-scoped
75
(b) Extended analyzer
point / structural
194
bound ≤ θ
75
needs shadow
66
bound > θ
60
lower bound
33
frame rule
23
summed bound
1
0
100
200
300
selected pairs (452 per analyzer)