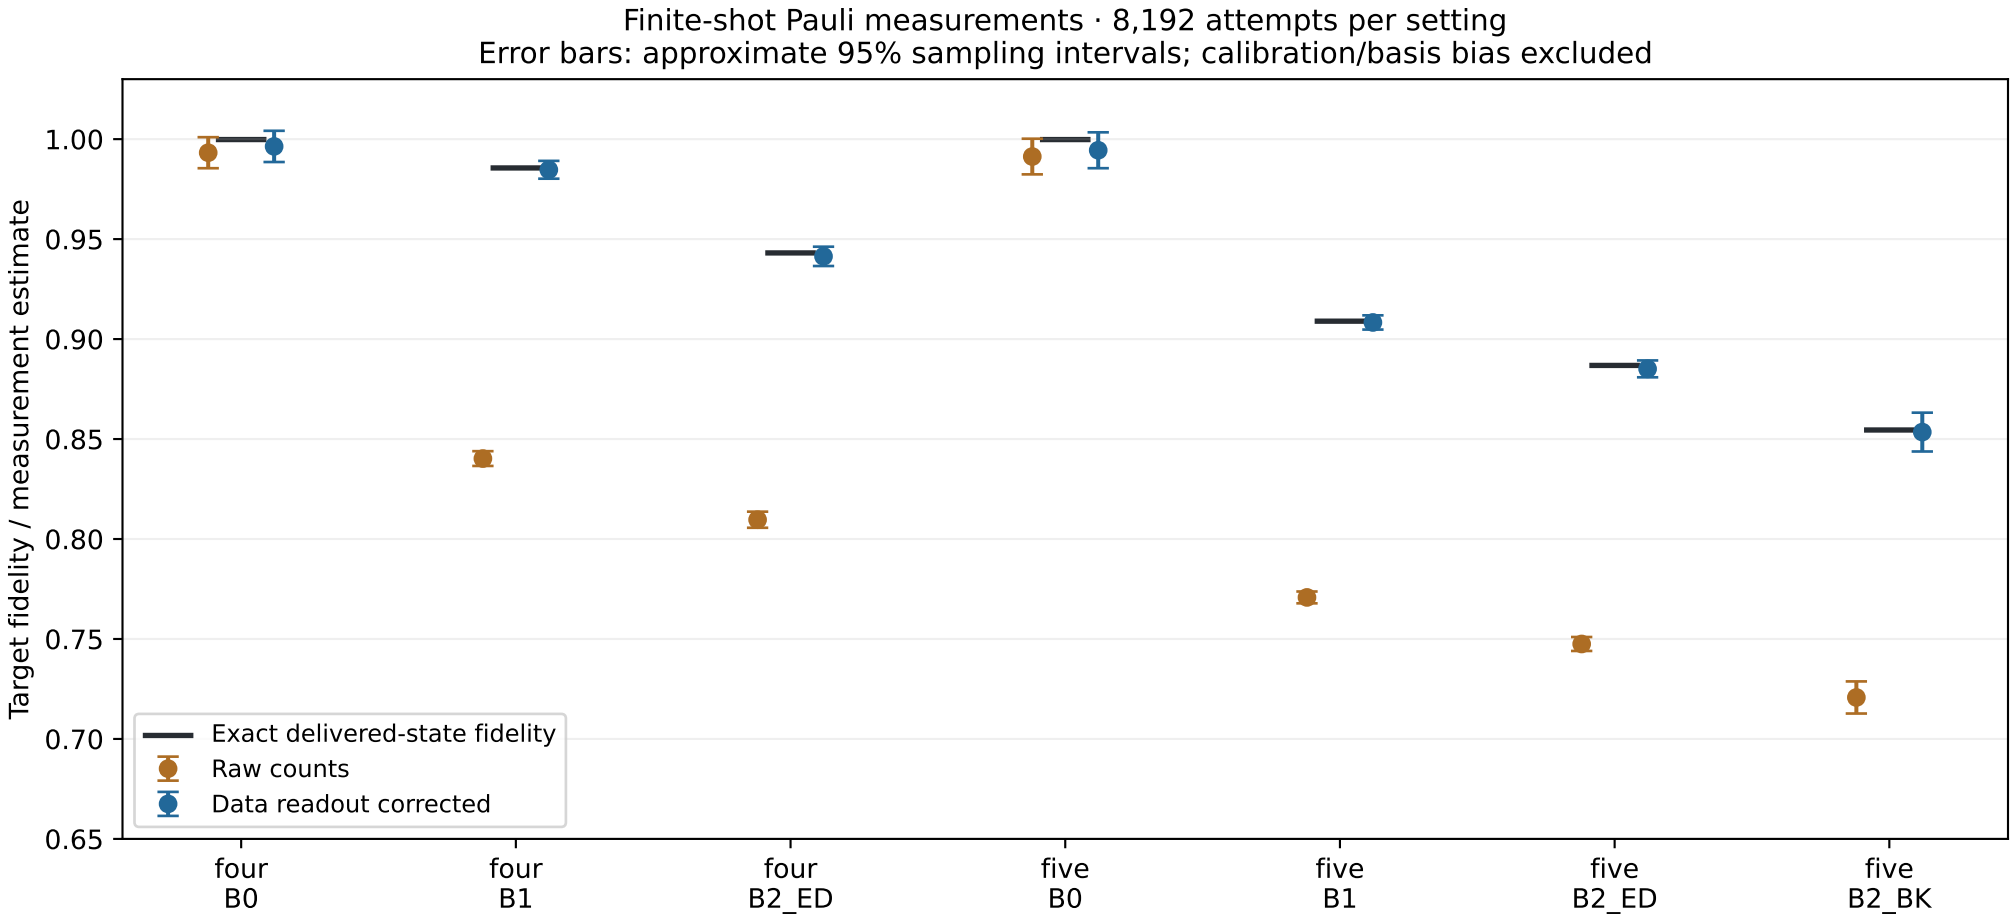
Finite-shot Pauli measurements · 8,192 attempts per setting
Error bars: approximate 95% sampling intervals; calibration/basis bias excluded
Target fidelity / measurement estimate
1.00
0.95
0.90
0.85
0.80
0.75
0.70
0.65
Exact delivered-state fidelity
Raw counts
Data readout corrected
four B0
four B1
four B2_ED
five B0
five B1
five B2_ED
five B2_BK