Bruker BioSpin MRI

ParaVision 360 V3.6

Reference Power Adjustment

- TX Coil: RF RES 400 1H 112/086 QSN
TO AD / RF ARR 400 1H M.BR. 2x2 RO AD

Table of Contents

1. Summary 2
2. Acquisition Information 2
3. Adjustment Progression 3
4. Profiles 7

1. Summary

Warnings:

No warnings.

Table 1. Results

Parameter	Value
PVM_StudyRefPow	2.037 W
Reference Power Status	Adj by Bruker:AdjRefPowADJ_REF_POW
Adjustment Status	Succeeded!

2. Acquisition Information

Table 2. Protocol Parameters

Parameter	Value
Method	Bruker:AdjRefPow
Nucleus	1H
Excitation Pulse Length	0.5 ms
Excitation Pulse Bandwidth	2,560 ms
Excitation Pulse Shape	bp.exc
Derive Init. Power	true
Nominal Init. FlipAngle	10
Adjustment Precision	0.3 dB
Initial Power	0.099 W
Max Power	471.366 W
Calculated Shape	false
Excitation Pulse Shape	bp.exc
Slice Thickness	5 mm
SliceOri	axial
Repetition Time	1,000 ms
Echo Time	15 ms
N Receive Channels	4
Channel Combination	AddImages

Table 3. Coil information

Parameter	Value
Coil configuration	RF RES 400 1H 112/086 QSN TO AD / RF ARR 400 1H M.BR. 2x2 RO AD
Operation Mode	[1H] TX Volume Array, RX Surface Array

Parameter	Value
Active Tx Coil	1
Tx Coil Status Ch1	System (Coil)
Tx Amp Scaling 1	100
Tx Phase Offset 1	0
Tx Amp Scaling 2	100
Tx Phase Offset 2	90
Tx Coil Element 1 active	true
Tx Coil Element 2 active	true
Active Rx Coil	1
Active Receivers	4
Rx Coil Element 1 active	true
Rx Coil Element 2 active	true
Rx Coil Element 3 active	true
Rx Coil Element 4 active	true

Routing Information

$Bis,1,20241031,2048,ROUTING,2#$Name,[1H] TX Volume Array, RX Surface Array# $OpMode,1.0,D/A,2.16.756.5.5.200.8323328.8454.1730396294.34#$TxCoil,1.0,1,RF RES 400 1H 112/086 QSN TO AD,BMRIDE,T12054V3,0120,1-2#$RxCoil,1.0,1,RF ARR 400 1H M.BR. 2x2 RO AD,BMRIDE,T11071V3,0093,1-4#$RfConn,1.0, Chan,1, Nuc,1H#$RfConn,1.0, Chan,1, TxSgu,2/3#$RfConn,1.0, TxSgu,2/3, Amp,2/3#$RfConn,1.0, Amp,2/3, TxPreamp,3/4#$RfConn,1.0, Chan,1, RxSgu,4/5/6/7#$RfConn,1.0, RxSgu,4/5/6/7, Rec,4/5/6/7#$RfDevProp,1.0, Amp,2/3, HpMode,On##$EndBis,9A,1D#

3. Adjustment Progression

Figure 1. Spin Echo Phase Channel 1

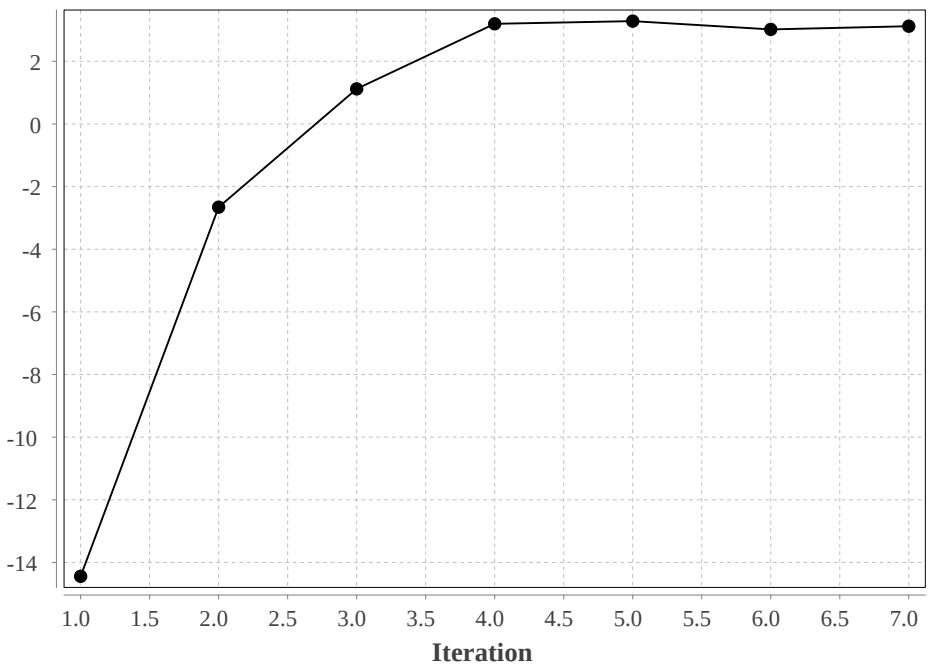

Figure 2. Spin Echo Phase Channel 2

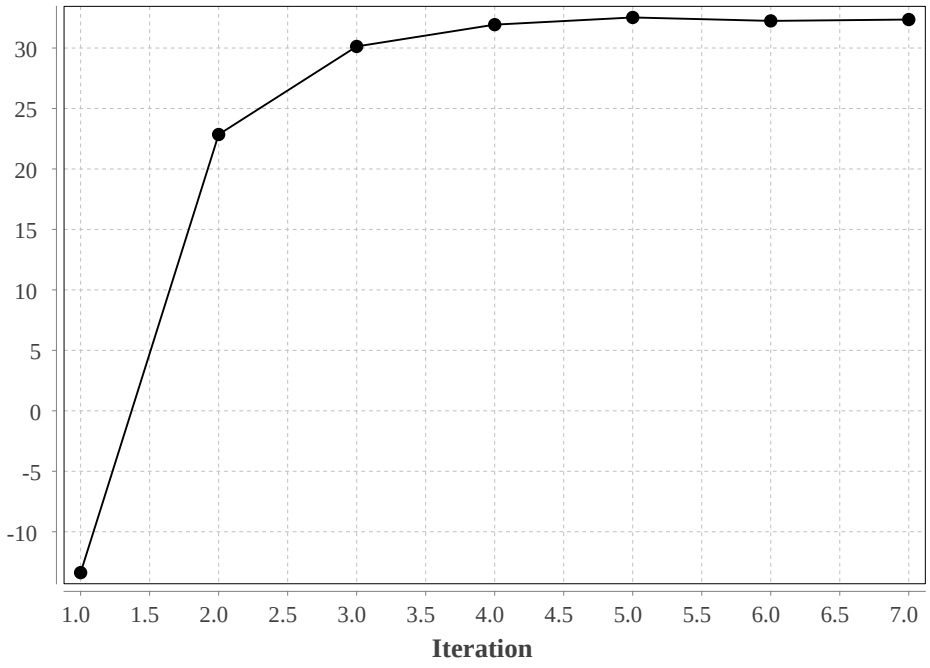

Figure 3. Spin Echo Phase Channel 3

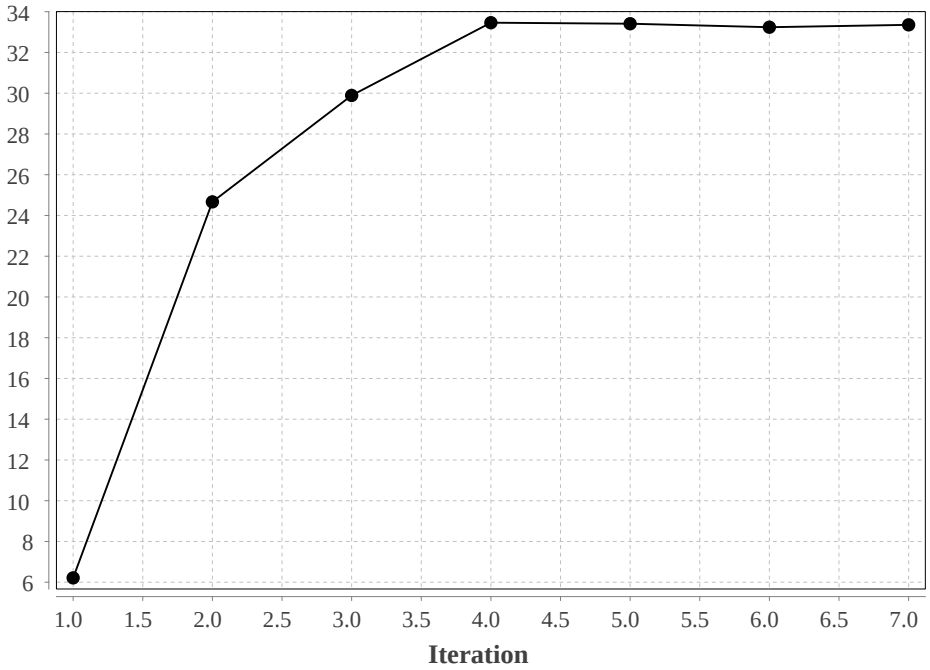

Figure 4. Spin Echo Phase Channel 4

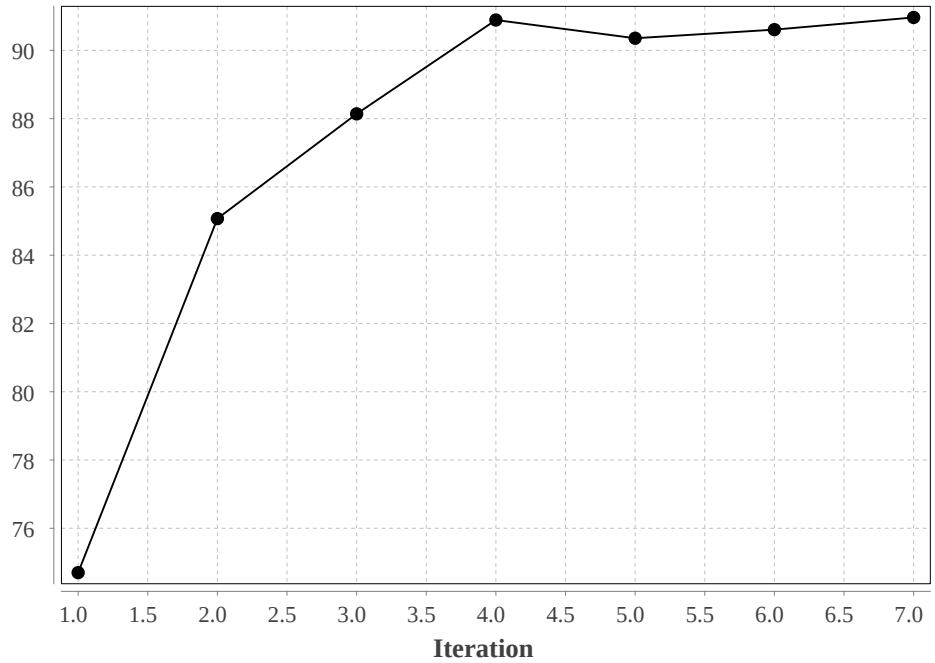

Figure 5. Pulse Power of Adjustment Pulse

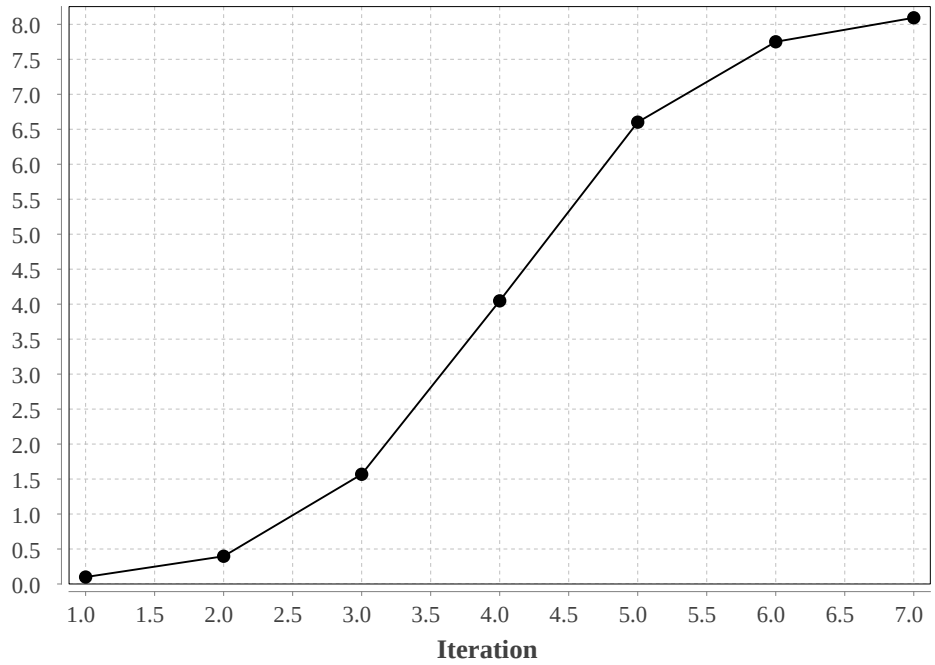

Figure 6. Receiver Gain

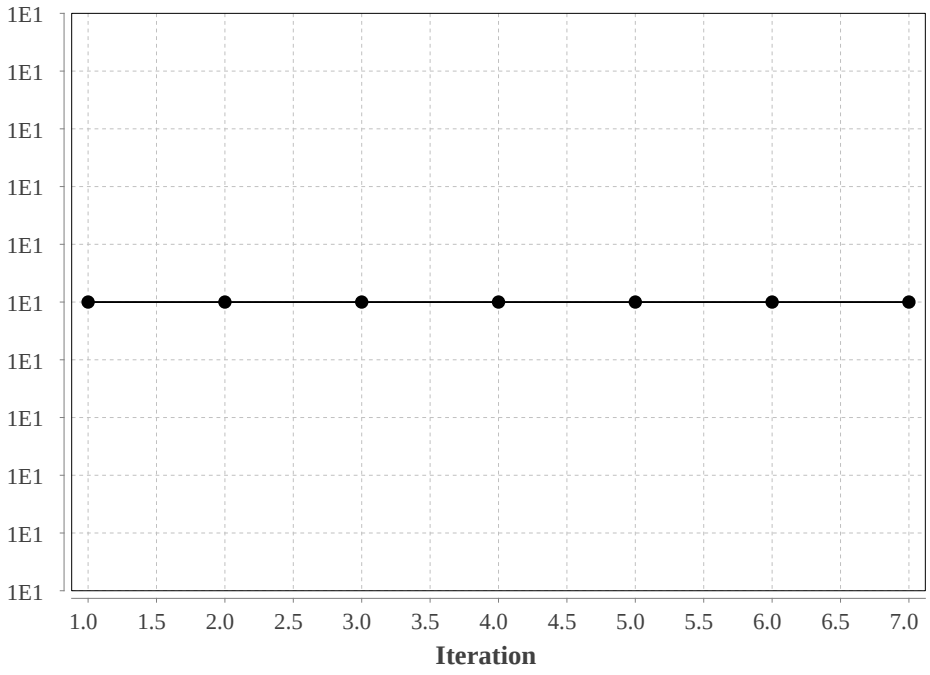

Figure 7. STE / SE ratio

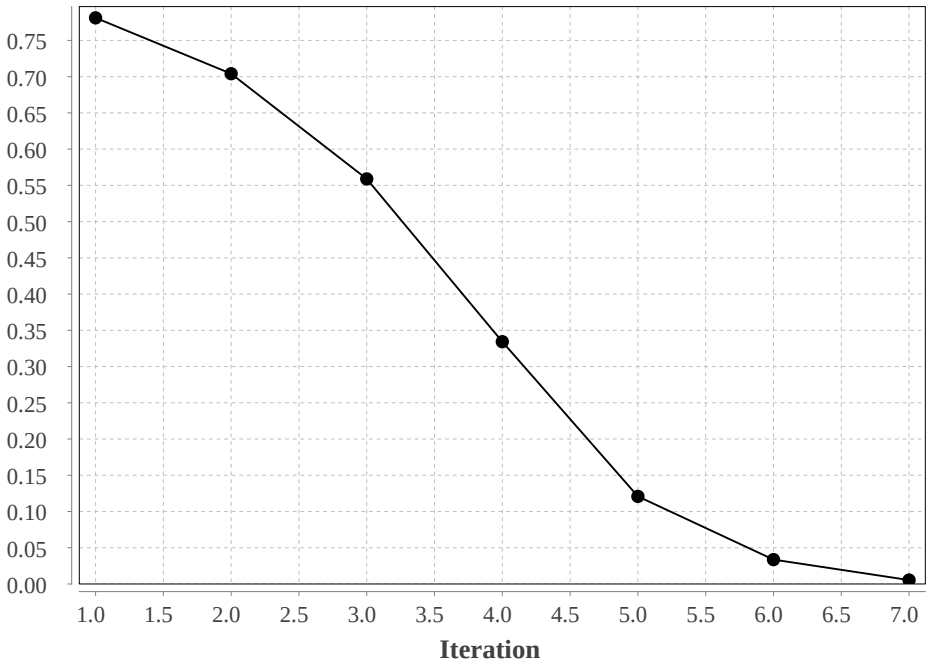

4. Profiles

Figure 8. Spin Echo Sum Profile (real part)

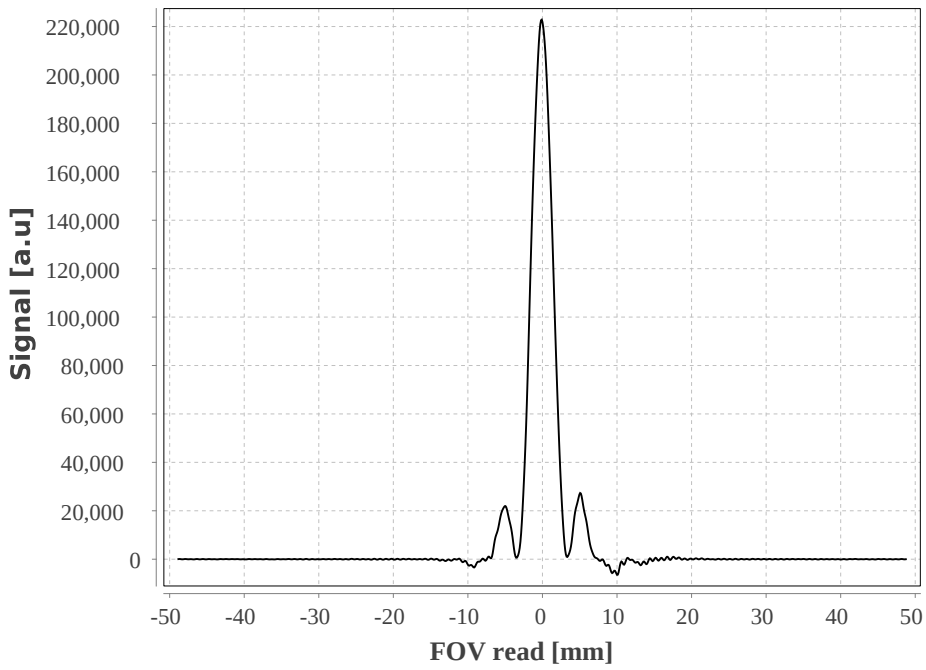

Figure 9. Spin Echo Sum Profile (imag part)

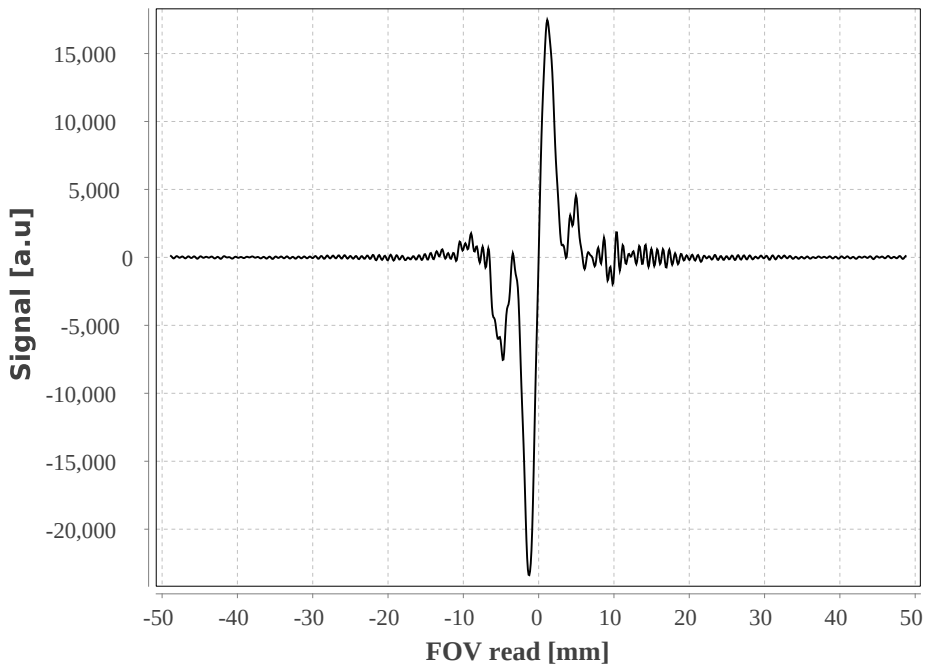

Figure 10. Stimulated Echo Sum Profile (real part)

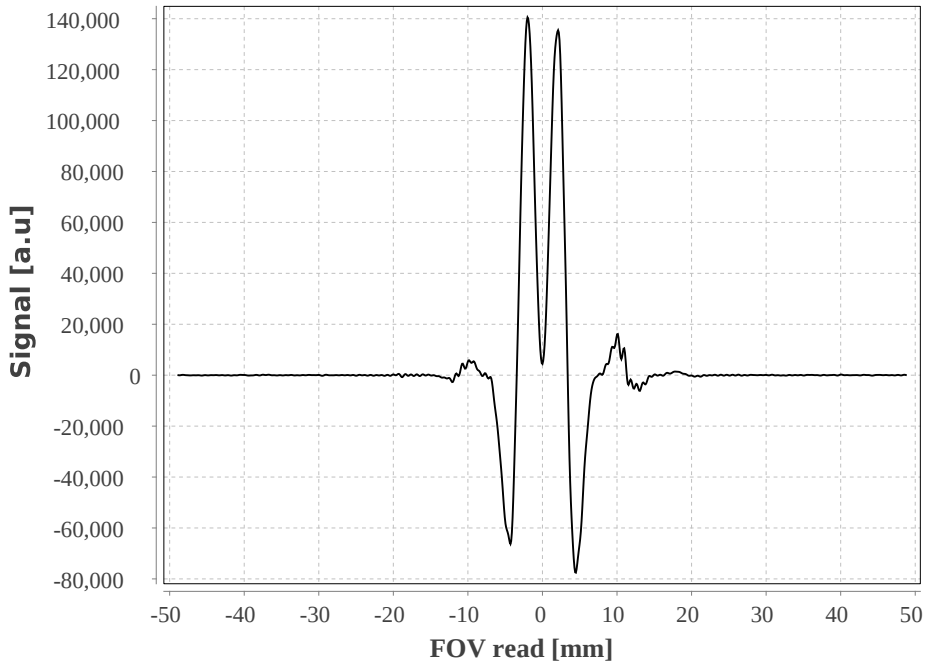

Figure 11. Stimulated Echo Sum Profile (imag part)

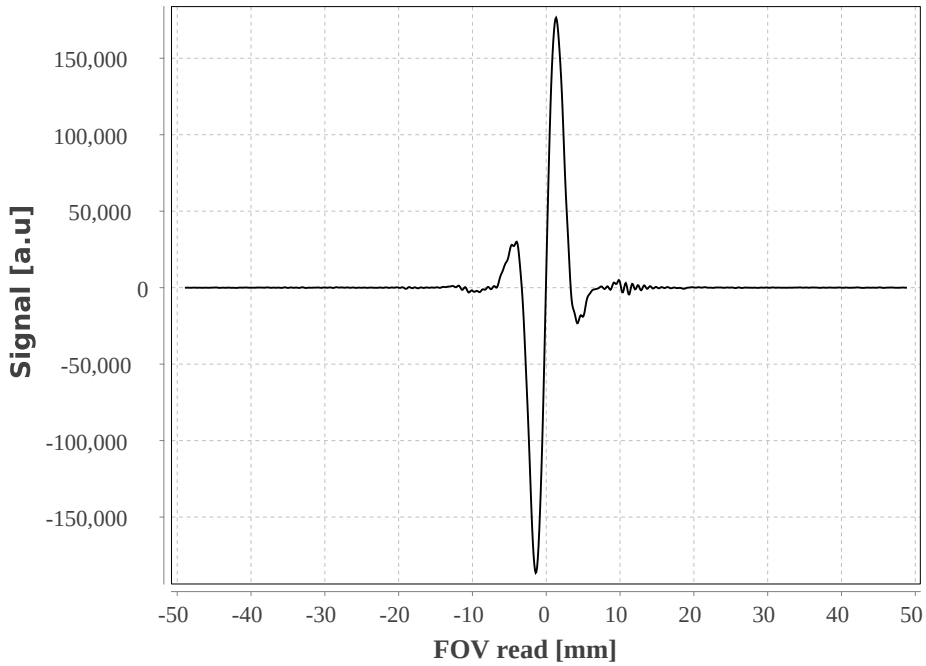

Figure 12. Spin Echo Profile (real part) channel 1

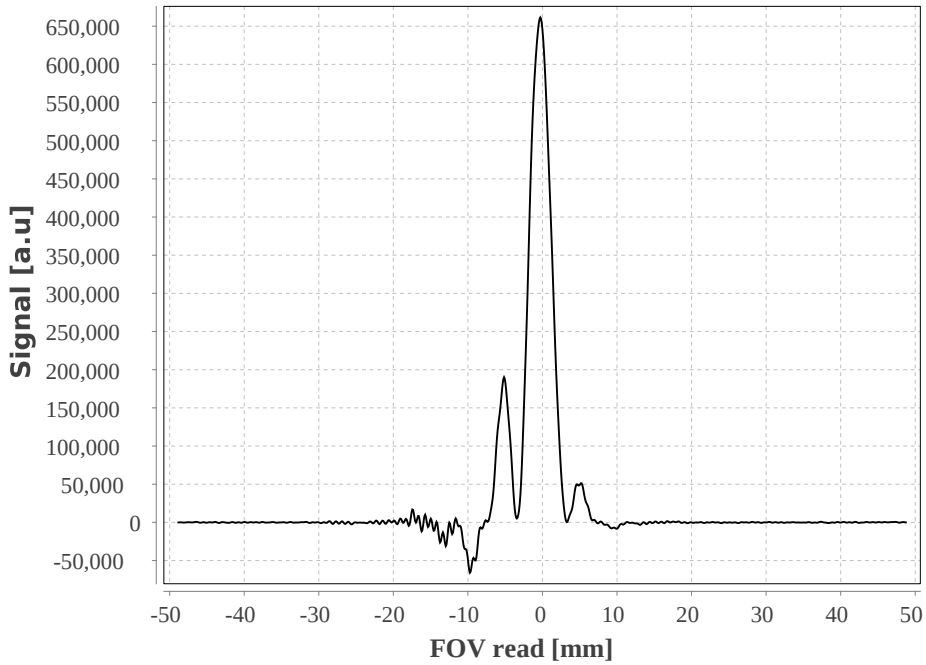

Figure 13. Spin Echo Profile (imag part) channel 1

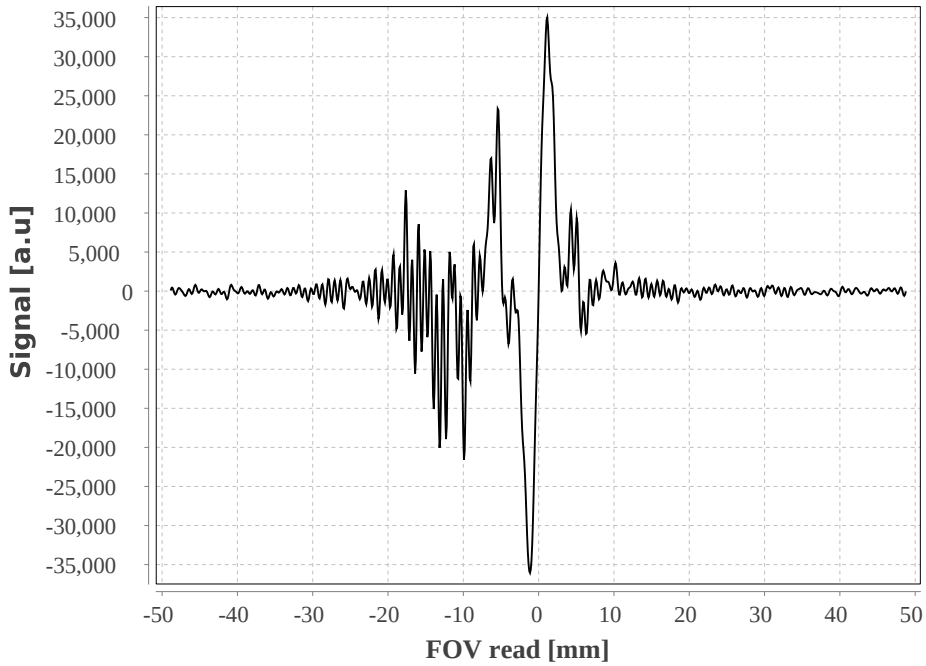

Figure 14. Stimulated Echo Profile (real part) channel 1

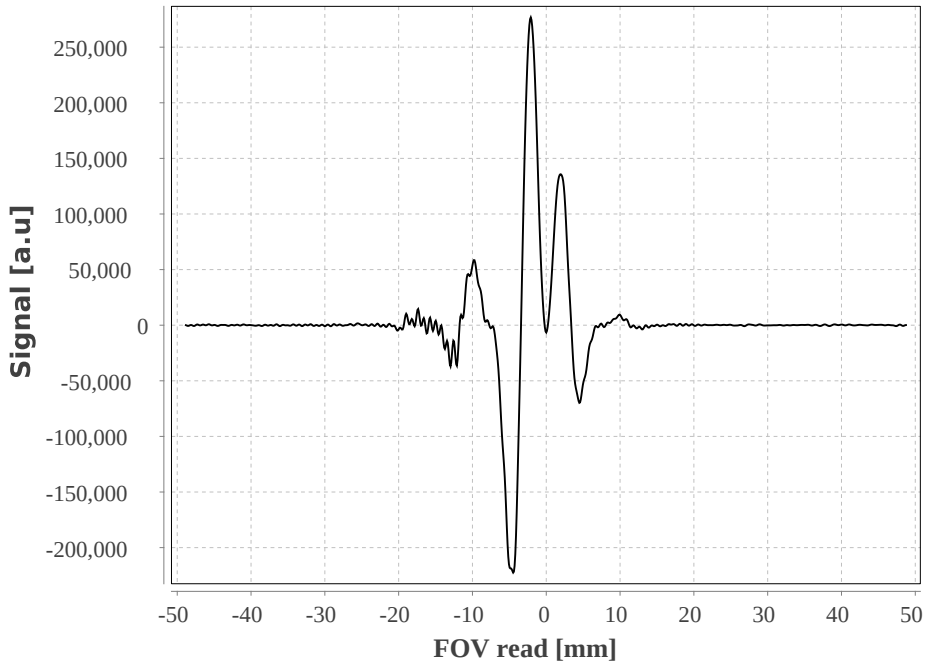

Figure 15. Stimulated Echo Profile (imag part) channel 1

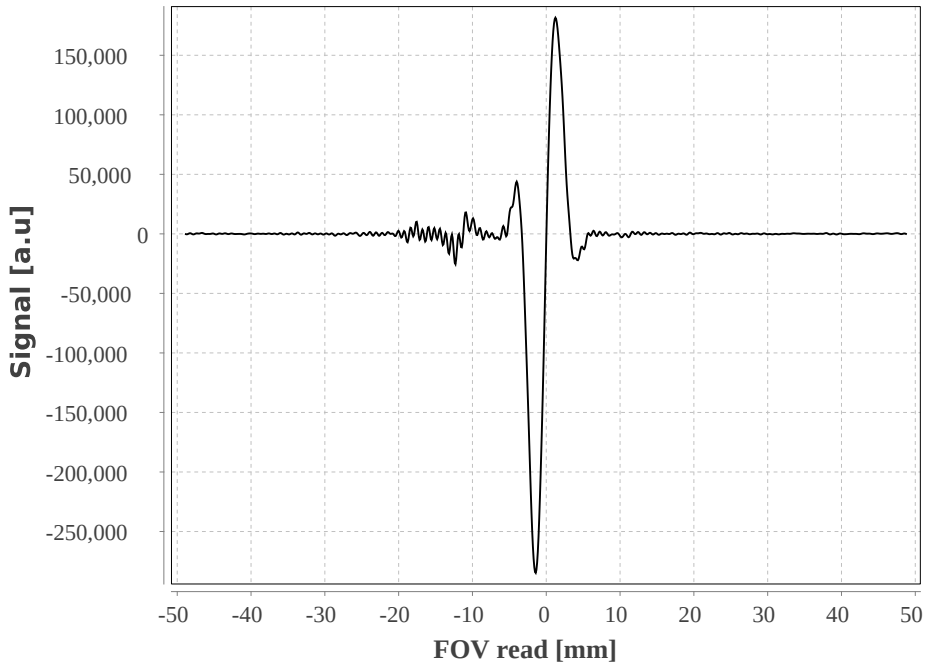

Figure 16. Spin Echo Profile (real part) channel 2

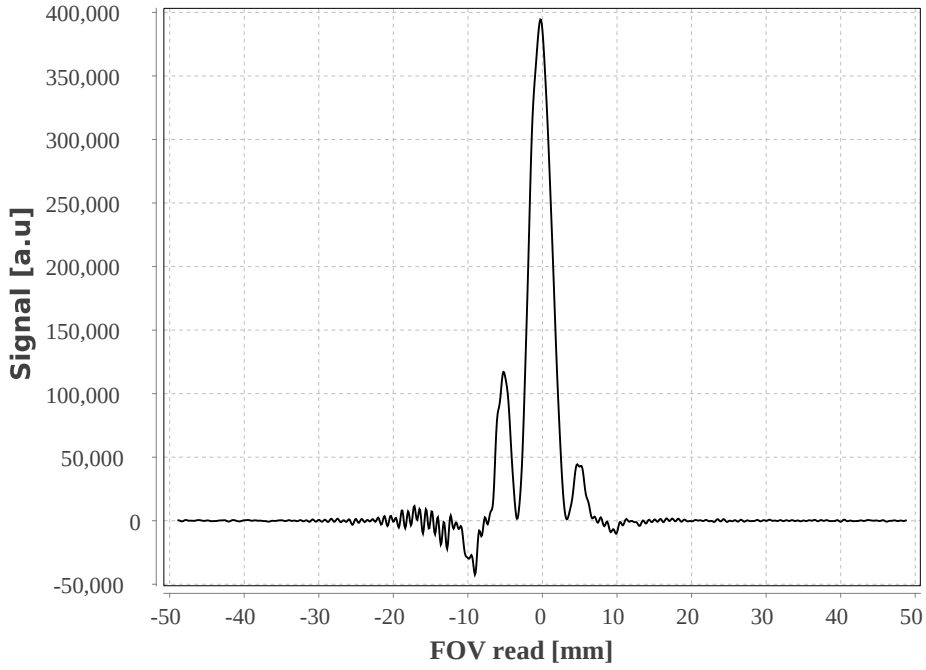

Figure 17. Spin Echo Profile (imag part) channel 2

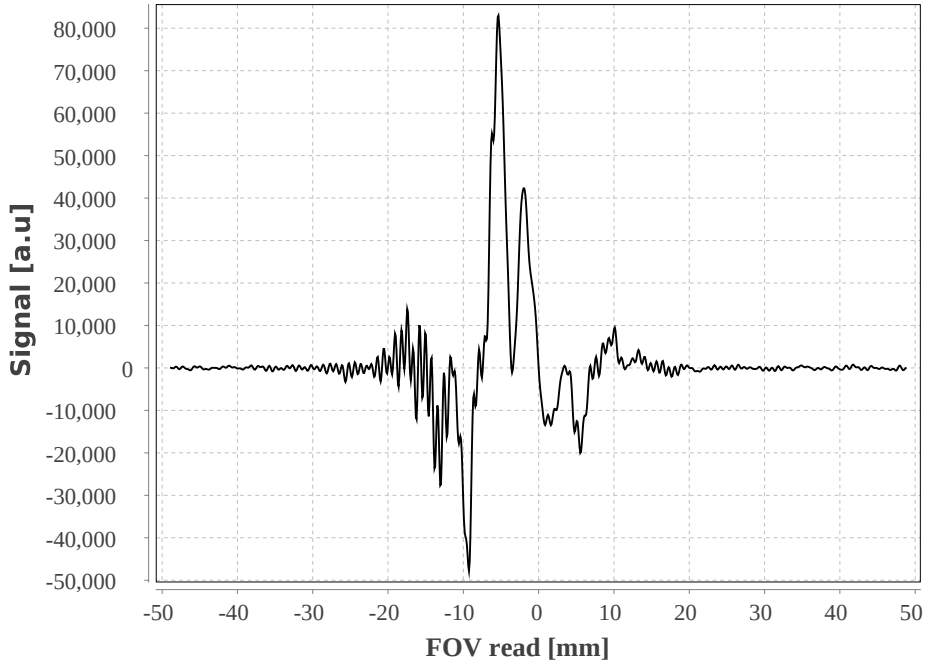

Figure 18. Stimulated Echo Profile (real part) channel 2

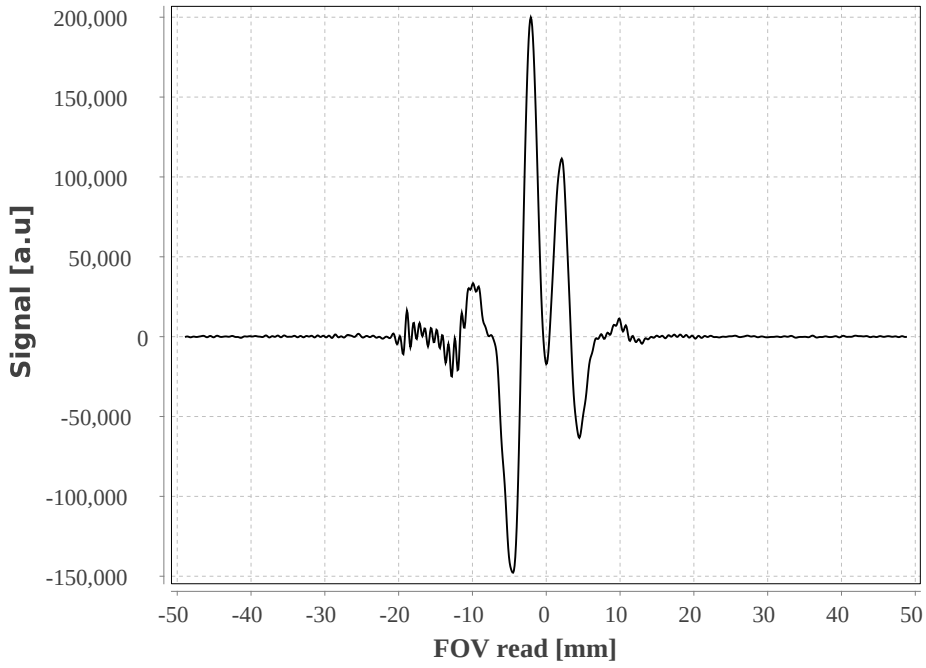

Figure 19. Stimulated Echo Profile (imag part) channel 2

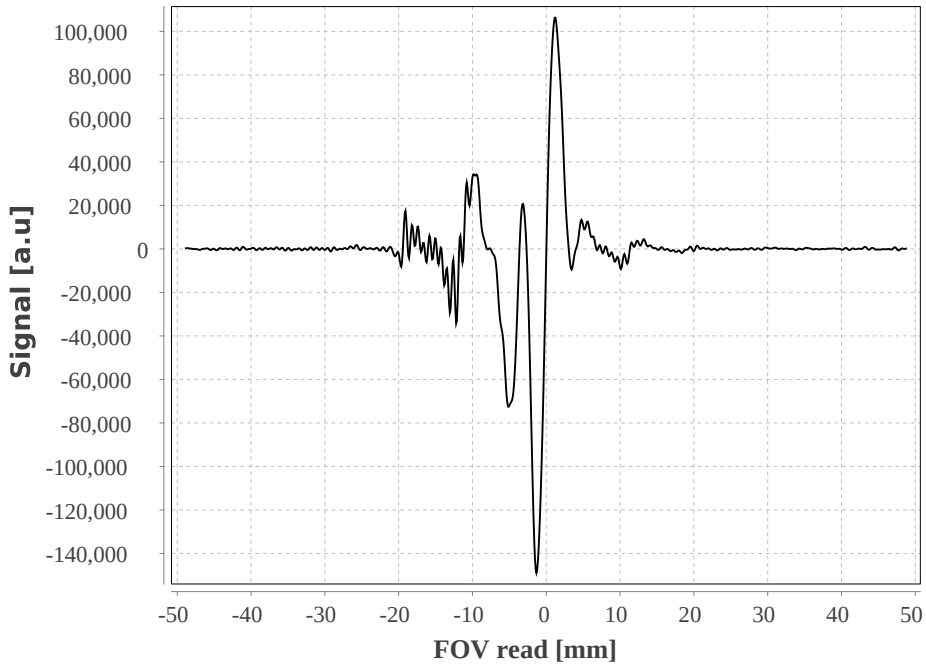

Figure 20. Spin Echo Profile (real part) channel 3

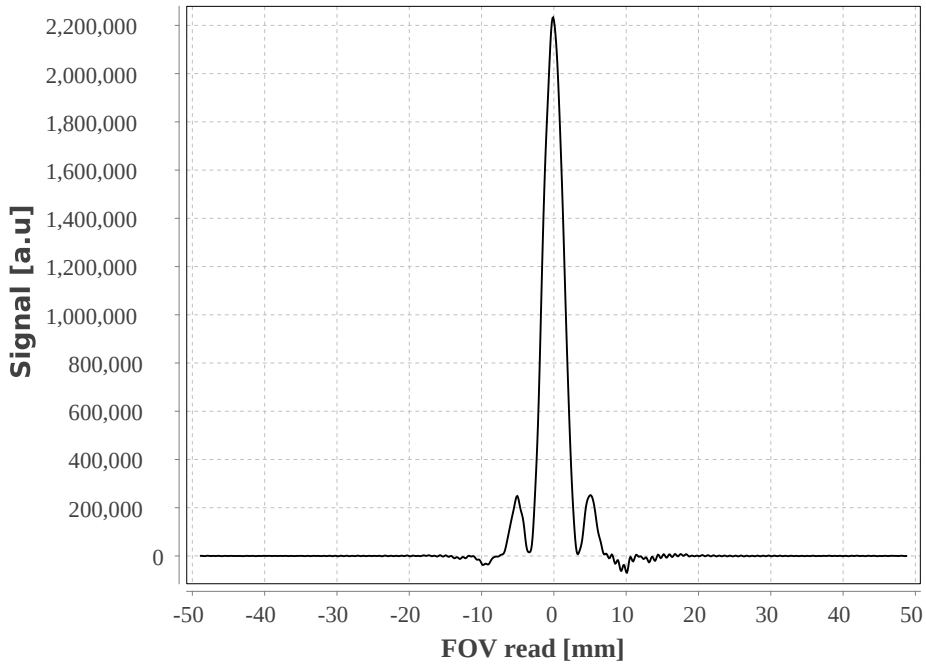

Figure 21. Spin Echo Profile (imag part) channel 3

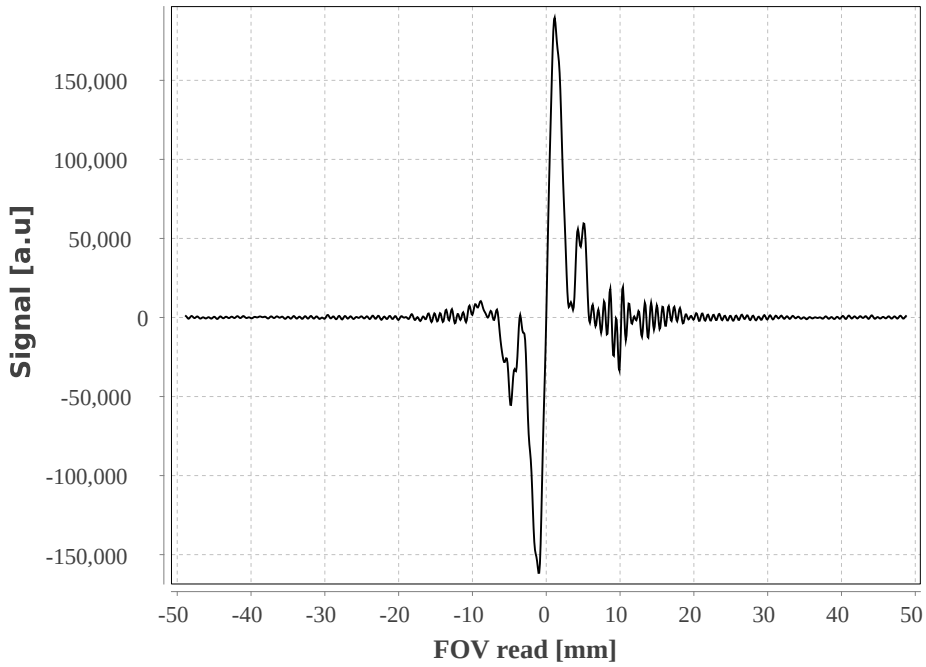

Figure 22. Stimulated Echo Profile (real part) channel 3

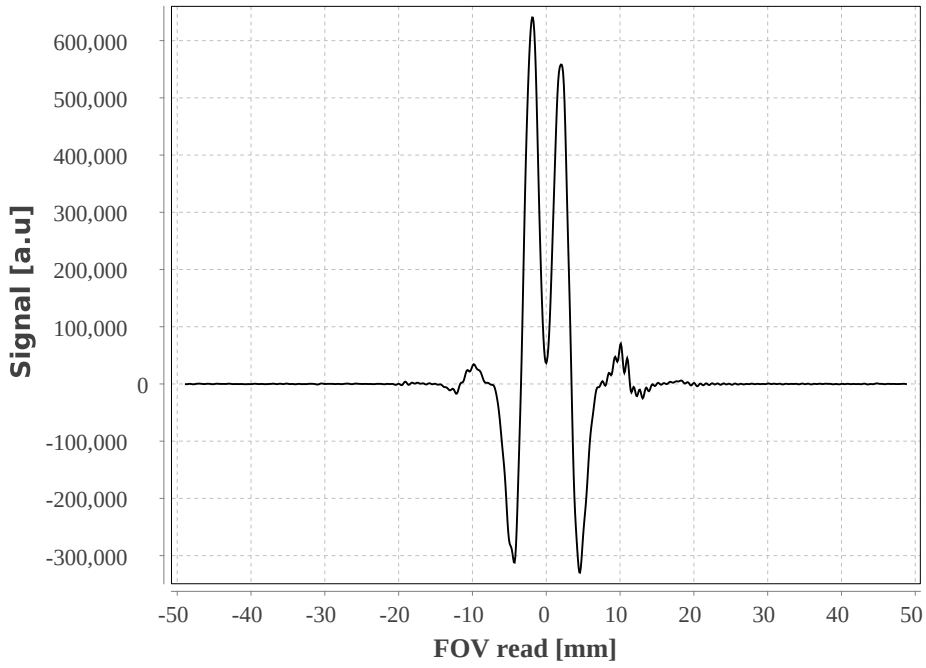

Figure 23. Stimulated Echo Profile (imag part) channel 3

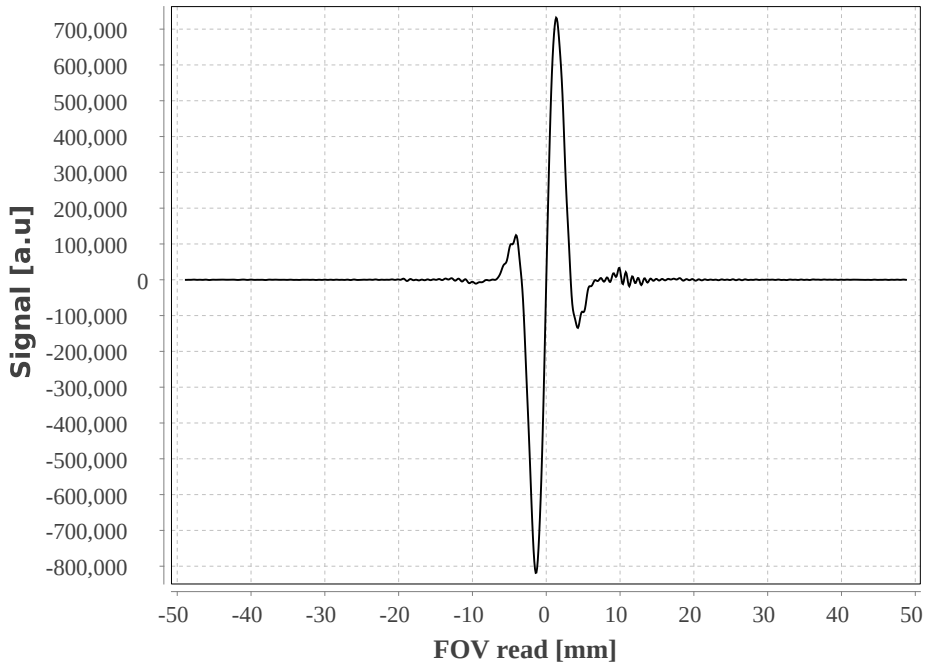

Figure 24. Spin Echo Profile (real part) channel 4

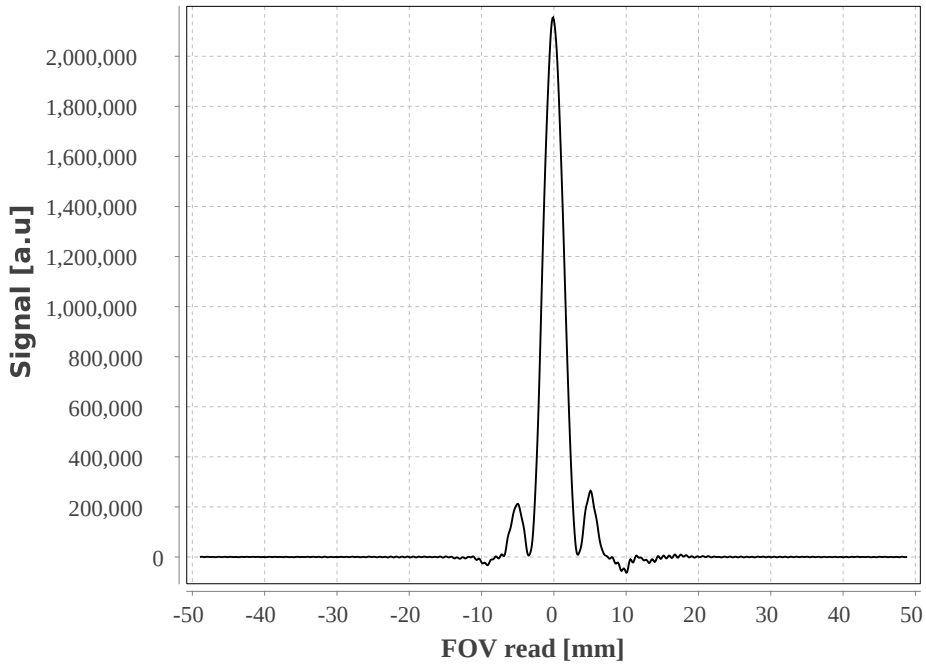

Figure 25. Spin Echo Profile (imag part) channel 4

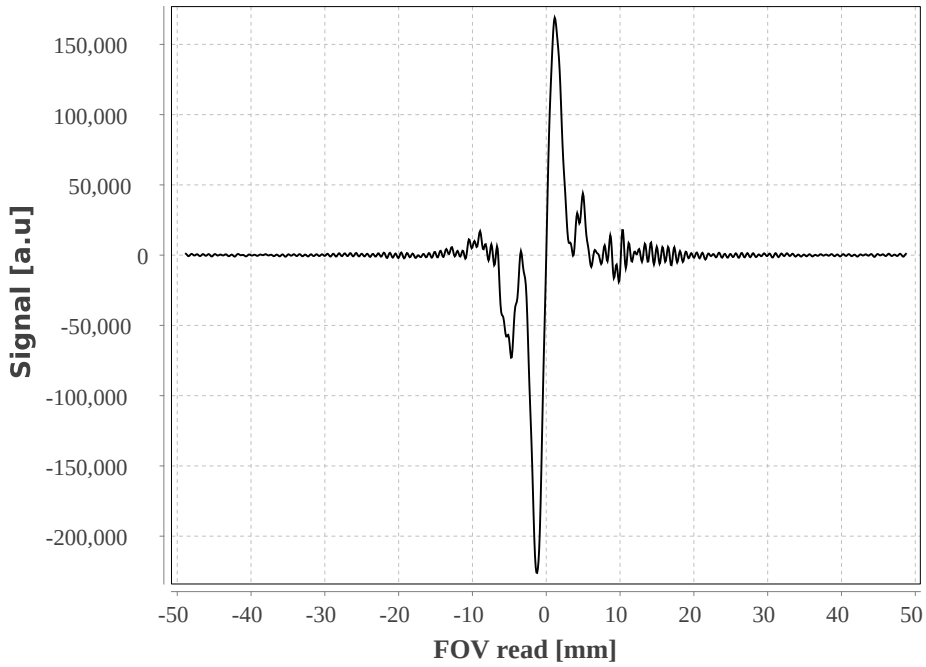

Figure 26. Stimulated Echo Profile (real part) channel 4

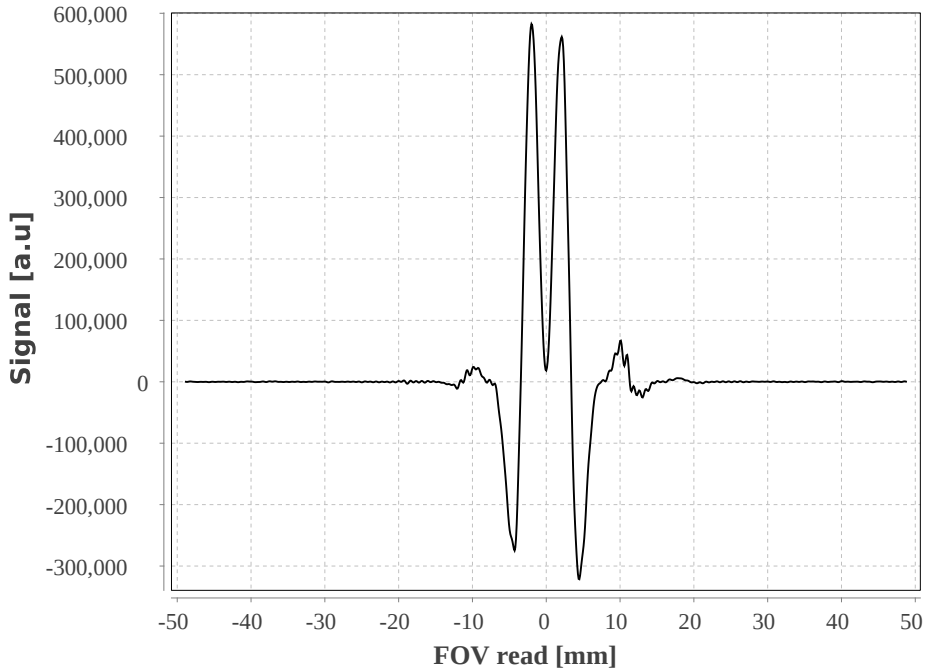
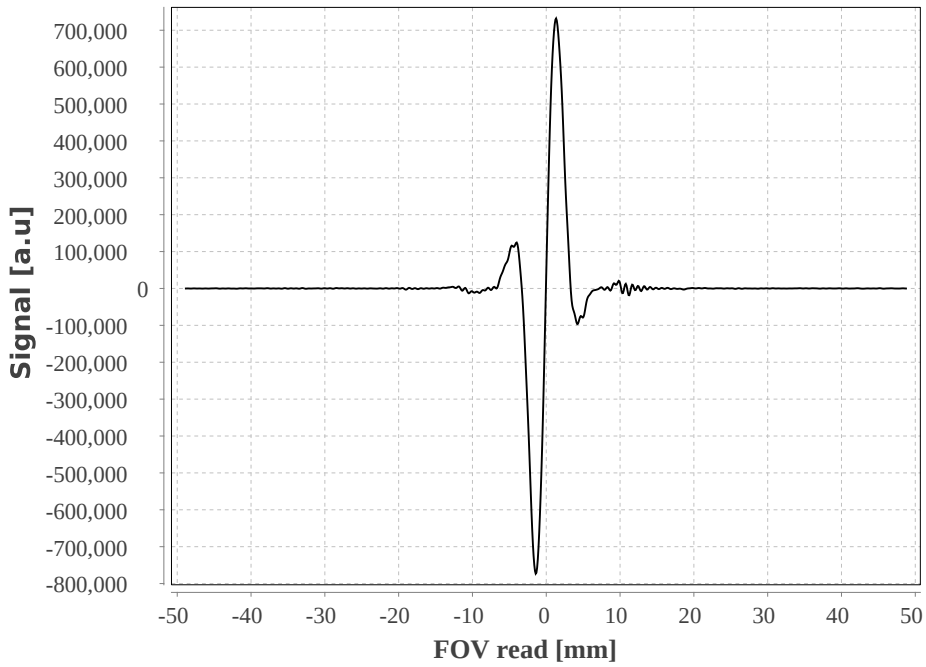
Figure 27. Stimulated Echo Profile (imag part) channel 4